

## Liquid chromatography-tandem mass spectrometry for monitoring vitamin D hydroxymetabolites in human aqueous humor

Neus Fabregat-Cabello<sup>a,\*</sup>, Pierre Darimont<sup>a</sup>, Loreen Huyghebaert<sup>a</sup>, Pascal Reynier<sup>b</sup>,  
Cédric Annweiler<sup>c,d</sup>, Dan Milea<sup>e,f</sup>, Caroline Le Goff<sup>a</sup> and Étienne Cavalier<sup>a</sup>.

<sup>a</sup> Department of Clinical Chemistry, University of Liège, CHU Sart-Tilman, Liège, Belgium

<sup>b</sup> Department of Biochemistry and Genetics, CHU d'Angers, Angers, France

<sup>c</sup> Department of Geriatric Medicine, Angers University Hospital; Research Center on Autonomy and Longevity; University Memory Clinic of Angers; UPRES EA 4638, University of Angers, Angers, France

<sup>d</sup> Robarts Research Institute, Department of Medical Biophysics, Schulich School of Medicine and Dentistry, the University of Western Ontario, London, Ontario, Canada

<sup>e</sup> Department of Ophthalmology, Angers University Hospital, Angers, France

<sup>f</sup> Singapore Eye Research Institute; Singapore National Eye Centre, and Duke-NUS, Neuroscience and Behavioral Diseases, Singapore

\*Author Present address

Neus Fabregat-Cabello, Hematology and Hemotherapy group, Health Research Institute Hospital La Fe (IIS La Fe), Valencia, Spain

\*Corresponding author:

Neus Fabregat-Cabello, Ph.D., Hematology and Hemotherapy group, Health Research Institute Hospital La Fe (IIS La Fe), Valencia, Spain, Phone: +34 96 12 46692, Fax: +34 96 124 66 20, E-mail: N.Fabregat@outlook.es

Calibration for 24,25(OH)<sub>2</sub>D<sub>3</sub> Quanti:  $y = 13.16666x + 0.07492$  ( $r = 0.99809$ ) (weighting:  $1/x$ )

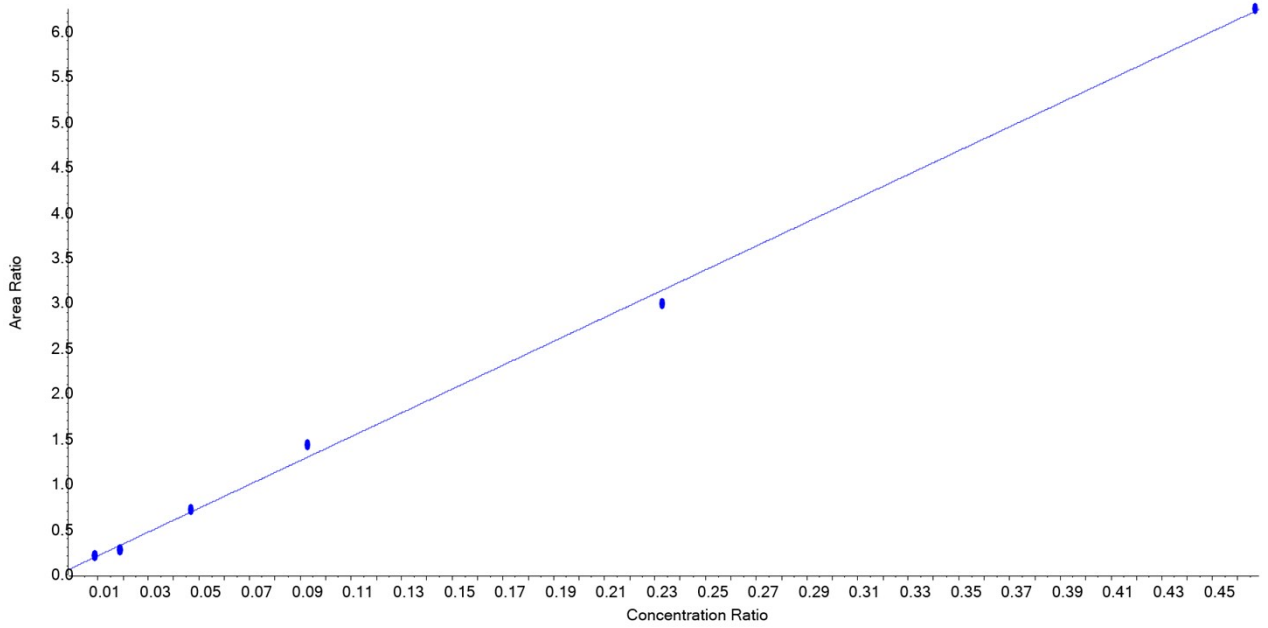


Figure S1. Calibration curve corresponding to the first day of validation for 24,25(OH)<sub>2</sub>D<sub>3</sub>,  $r=0,99809$ . Concentration in  $\mu\text{g/L}$ .

Calibration for 24,25(OH)<sub>2</sub>D<sub>2</sub> Quanti:  $y = 6.75545x + 0.01932$  ( $r = 0.99475$ ) (weighting:  $1/x$ )

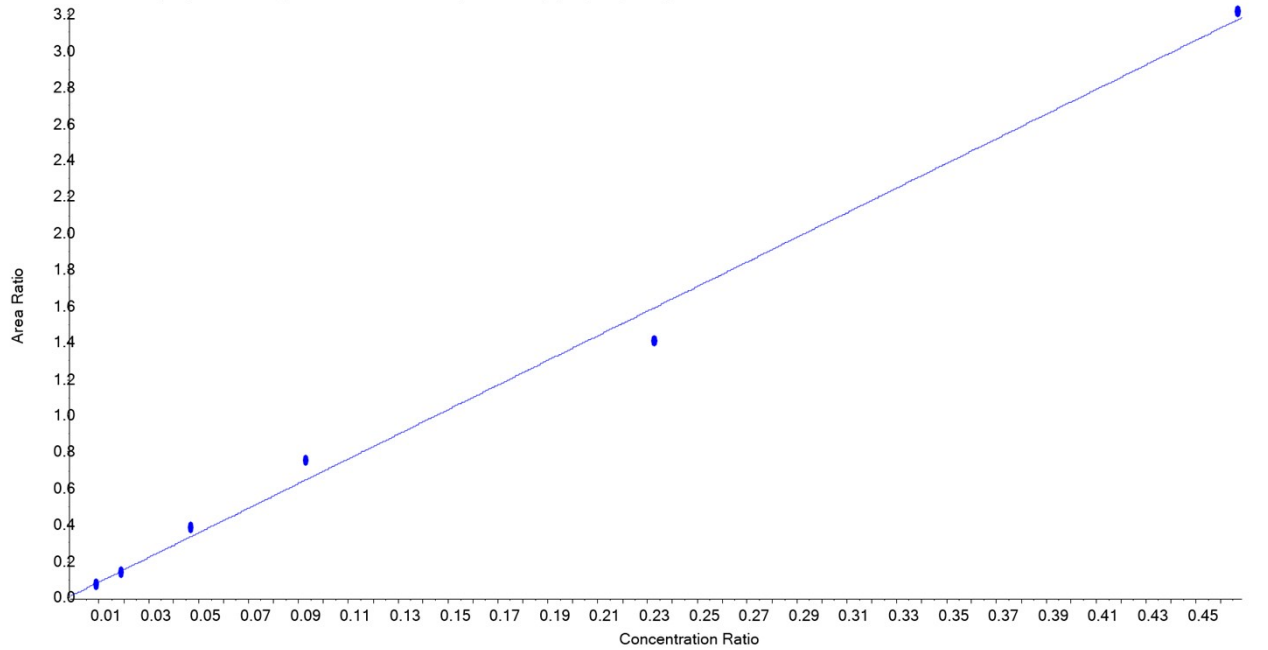


Figure S2. Calibration curve corresponding to the first day of validation for 24,25(OH)<sub>2</sub>D<sub>2</sub>,  $r=0,99475$ . Concentration in  $\mu\text{g/L}$ .

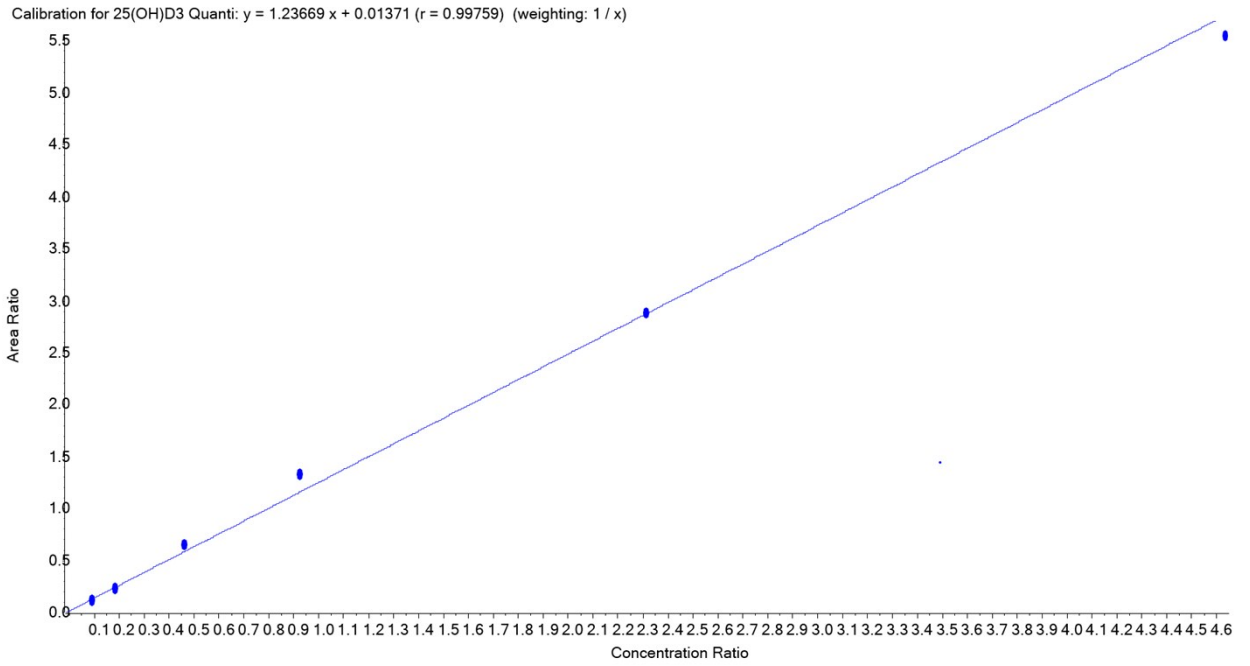


Figure S3. Calibration curve corresponding to the first day of validation for 25(OH)D<sub>3</sub>,  $r=0,99759$ . Concentration in  $\mu\text{g/L}$ .

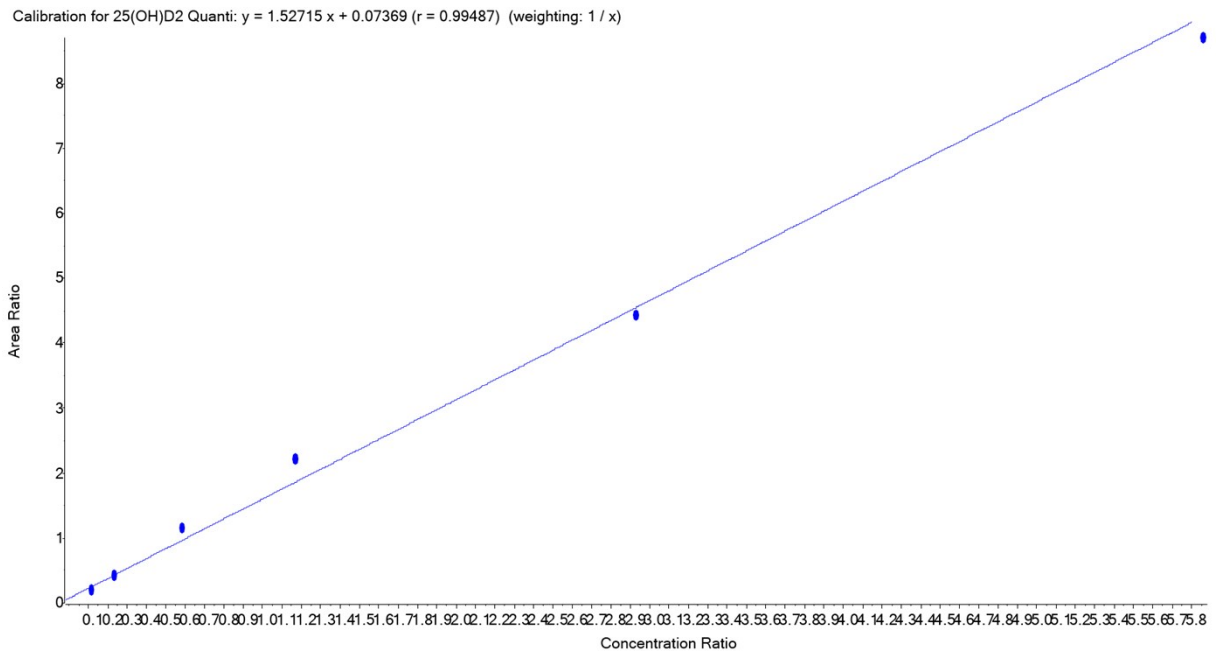


Figure S4. Calibration curve corresponding to the first day of validation for 25(OH)D<sub>2</sub>,  $r=0,99487$ . Concentration in  $\mu\text{g/L}$ .