

Fig. S1

TRU/DGA tandem column calibration

Recovery (%)

100
90
80
70
60
50
40
30
20
10
0

3M HCl 0.1M HNO₃ 0.05M HNO₃ 0.03M HNO₃ 0.006M HCl

Element

Mg
Ba
La
Ce
Pr
Nd
Sm
Gd
Yb
Lu

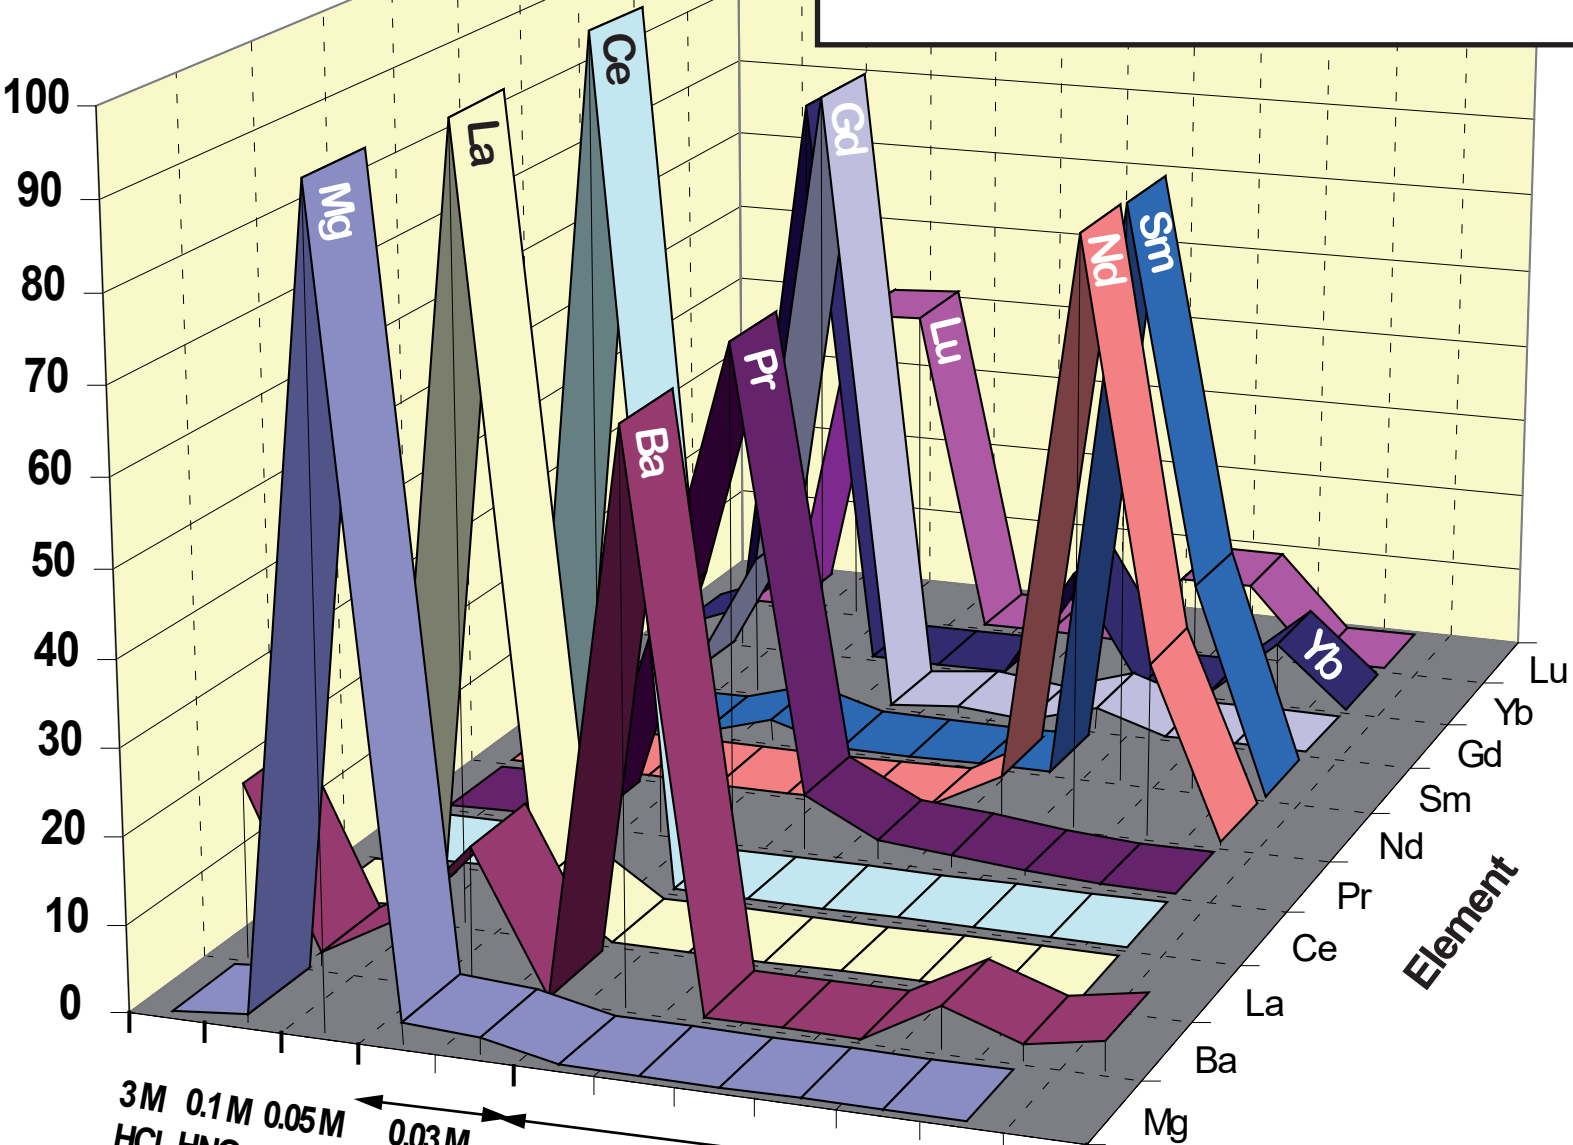


Fig. S2