

Supporting Information

SERS-based immunoassay using a gold array-embedded gradient microfluidic chip

Moonkwon Lee,^{†a} Kangsun Lee,^{†b} Ki Hyung Kim,^a

Kwang W. Oh^{*b} and Jaebum Choo^{*a}

^a*Department of Bionano Engineering, Hanyang University, Ansan 426-791, South Korea.*

E-mail: jbchoo@hanyang.ac.kr

^b*Department of Electrical Engineering, State University of New York at Buffalo, NY 14260,*

USA. E-mail: kwangoh@buffalo.edu

†Joint first authors

***Joint corresponding authors**

Address for correspondence:

Jaebum Choo

Telephone: +82-31-400-5201; Fax: +82-31-436-8188; E-mail: jbchoo@hanyang.ac.kr

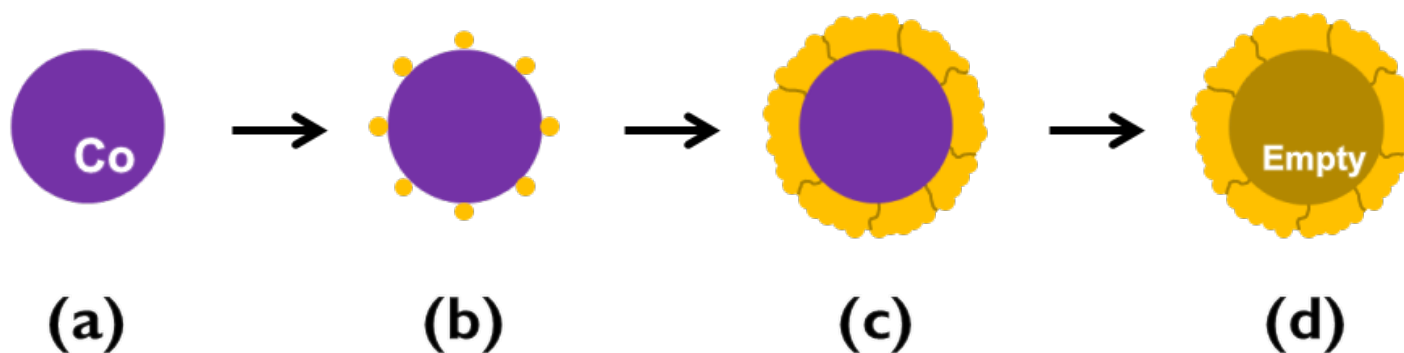


Figure S1. Fabrication process of hollow gold nanospheres (HGNs): (a) Synthesis of cobalt template, (b) Gold seeding, (c) Growth of the seeded gold, and (d) Oxidation of cobalt template and formation of HGN. A hollow interior is formed by dissolving the cobalt nanoparticle in the core.

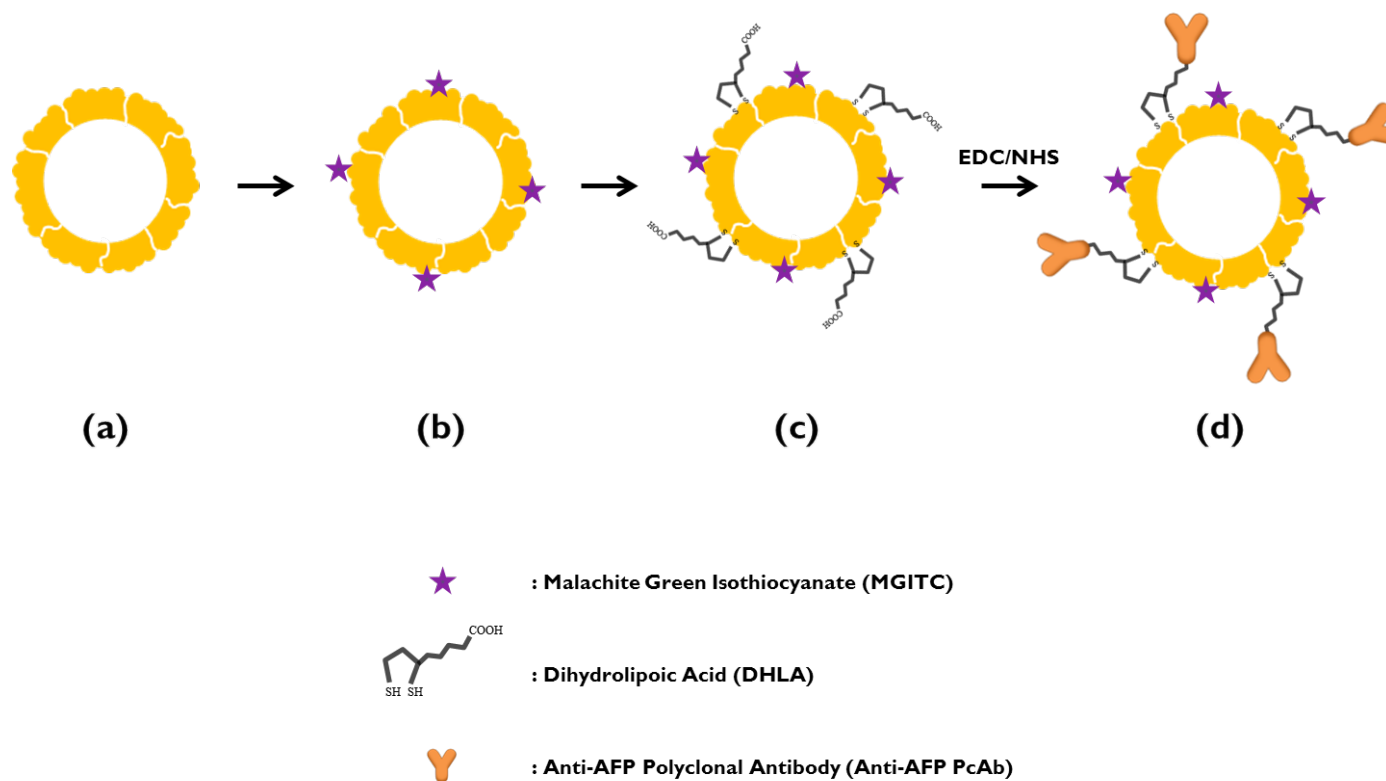


Figure S2. Antibody conjugation process on the fabricated hollow gold nanospheres (HGNs): (a) Fabricated HGN, (b) Adsorption of Raman reporter (Malachite green isothiocyanate, MGITC), (c) Activation of carboxylic acid group on the HGN, and (d) Conjugation of polyclonal antibody through EDC/NHS coupling chemistry.

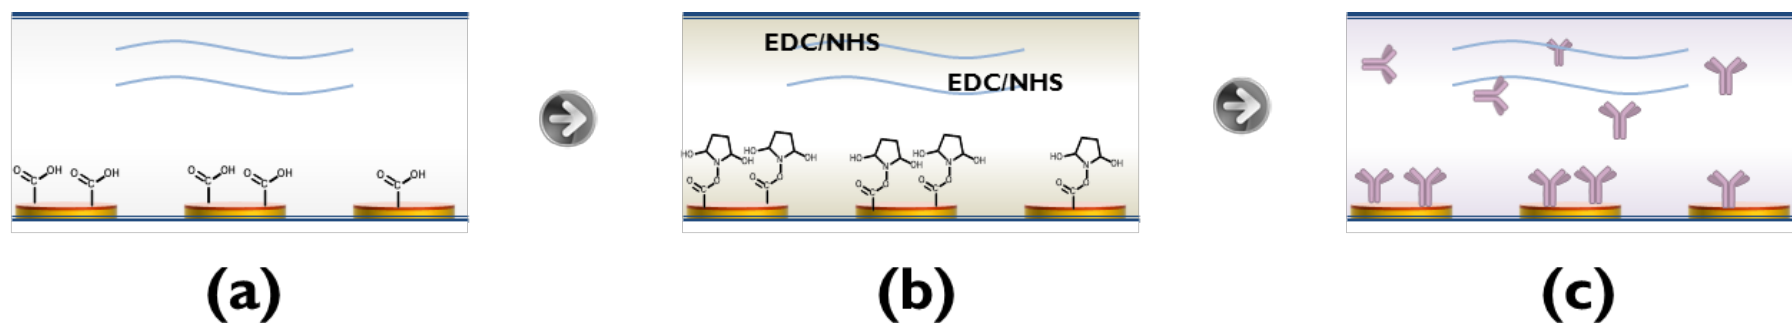


Figure S3. Schematic illustrations of the antibody conjugation process on the gold array wells embedded in a gradient microfluidic chip: (a) Preparation of carboxylic acid group on the gold array surface, (b) Activation of carboxylic acid group by NHS/EDC solution, and (c) Capture antibodies conjugation on the EDC-activated gold array surface.