


Supplementary Figure 1. Percentage loss of mass monitored over time as a result of evaporation of the normal clotting plasma sample applied to the open lateral flow channel device (n=3).

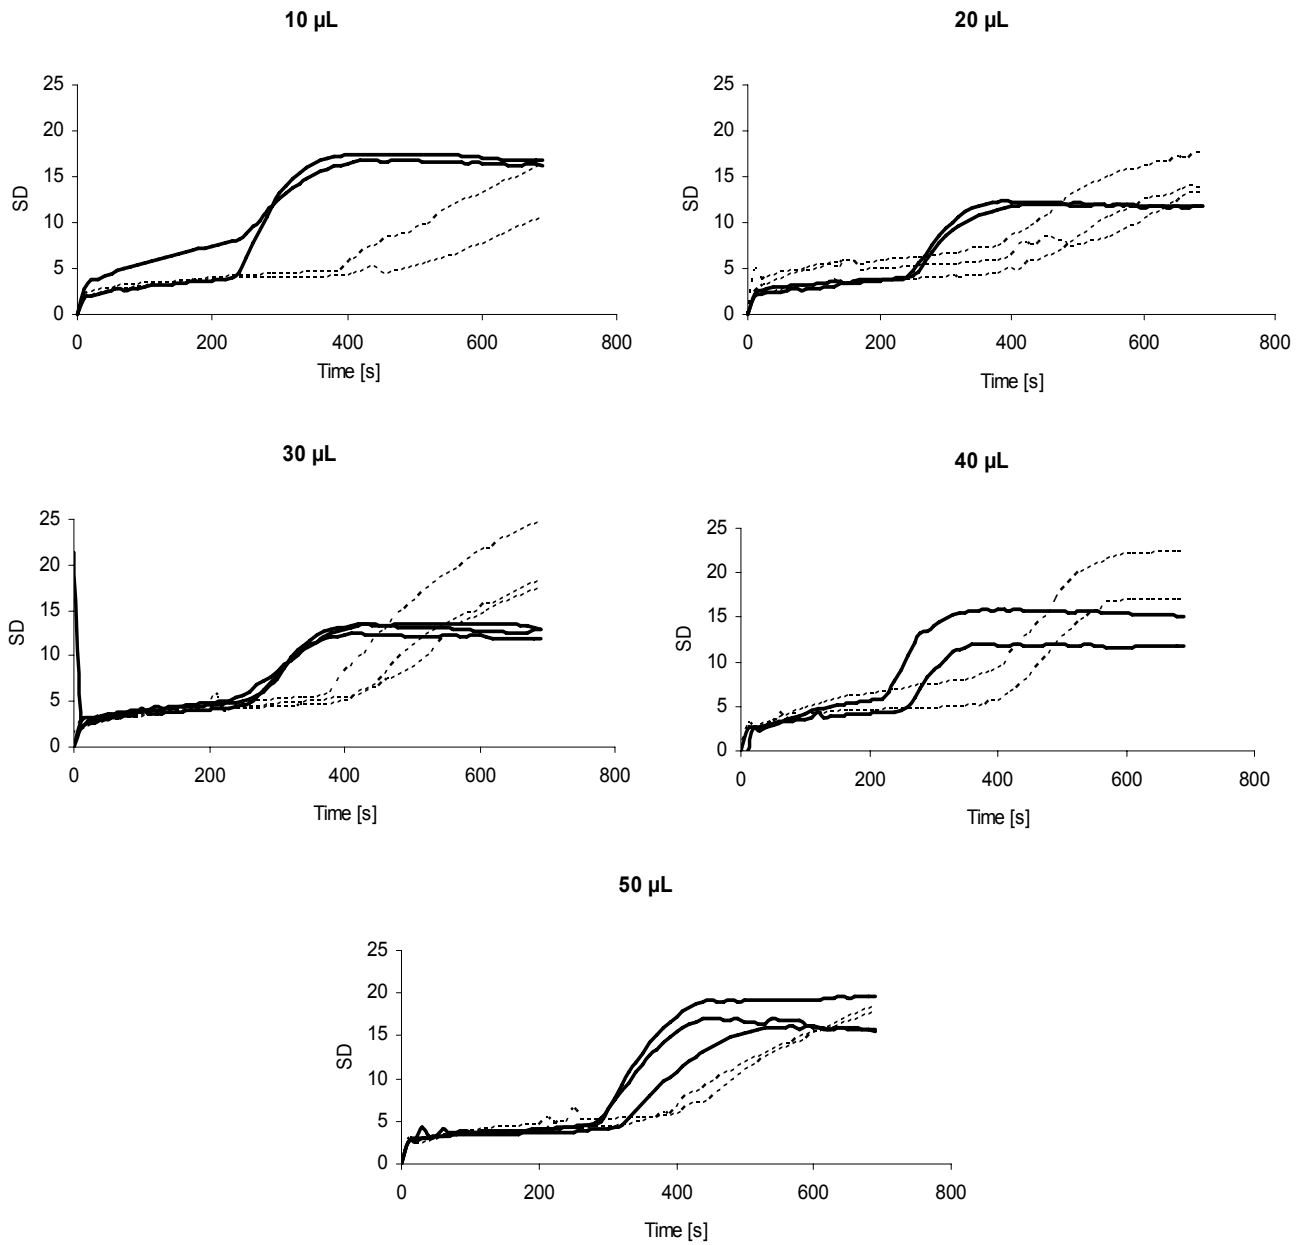

Supplementary Figure 2. Change in SD over time obtained for plasma spiked with 0 (solid line) and 0.5 U/mL of heparin (dotted line) tested in platforms where 10 – 50 μL of aPTT-SP were deposited and dried.