

Electronic Supporting Information (ESI) for

A ratiometric fluorescent metal ion indicator based on dansyl labeled poly(N-isopropylacrylamide) responds to a quenching metal ion

5
 Jie Du,^a Shaojun Yao,^a W. Rudolf Seitz,^{*a} Nicholas E. Bencivenga,^a Justin O. Massing,^a Roy P. Planalp,^a
 Randy K. Jackson,^b Daniel P. Kennedy^b and Shawn C. Burdette^b

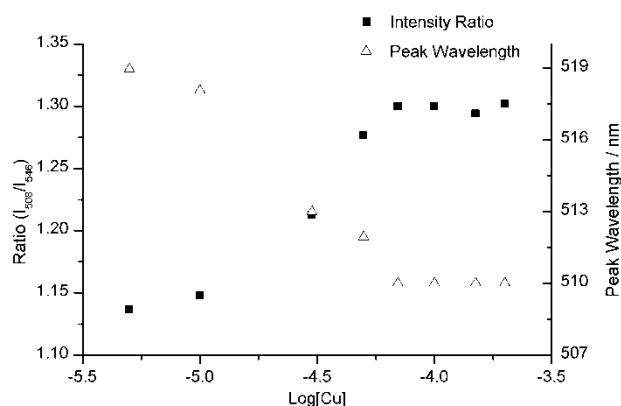


Fig. S1 Calibration curves for spectrofluorometric titration of Cu(II) indicator at 36 °C

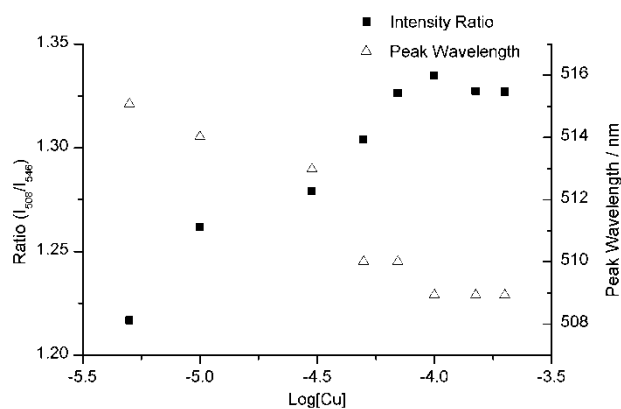


Fig. S2 Calibration curves for spectrofluorometric titration of Cu(II) indicator at 37 °C

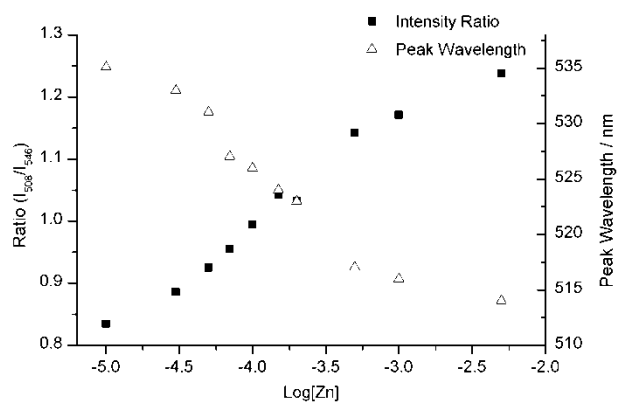


Fig. S3 Calibration curves for spectrofluorometric titration of indicator with Zn(II) at 35 °C

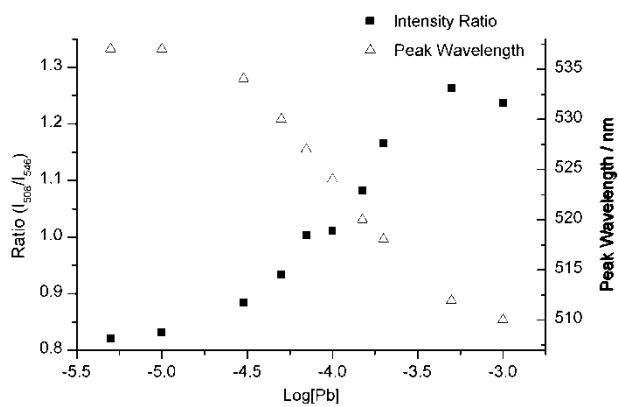


Fig. S4 Calibration curves for spectrofluorometric titration of indicator with Pb(II) at 35 °C