

Supplementary Figure

High Pressure Nano Electrospray Ionization Mass Spectrometry for Aqueous Solution

Md. Matiur Rahman¹, Mridul Kanti Mandal¹, Kenzo Hiraoka¹ and Lee Chuin Chen^{2*}

¹*Clean Energy Research Center, University of Yamanashi, 4-3-11, Takeda, Kofu, Yamanashi, 400-8511 Japan*


²*Interdisciplinary Graduate School of Medicine and Engineering, University of Yamanashi, 4-3-11, Takeda, Kofu, Yamanashi, 400-8511 Japan*

***Corresponding author:**

L.C. Chen, Tel: +8155-220-8072

Email: leechuin@yamanashi.ac.jp

Keywords: High pressure, Nano Electrospray, Aqueous solution, Corona discharge, Native protein

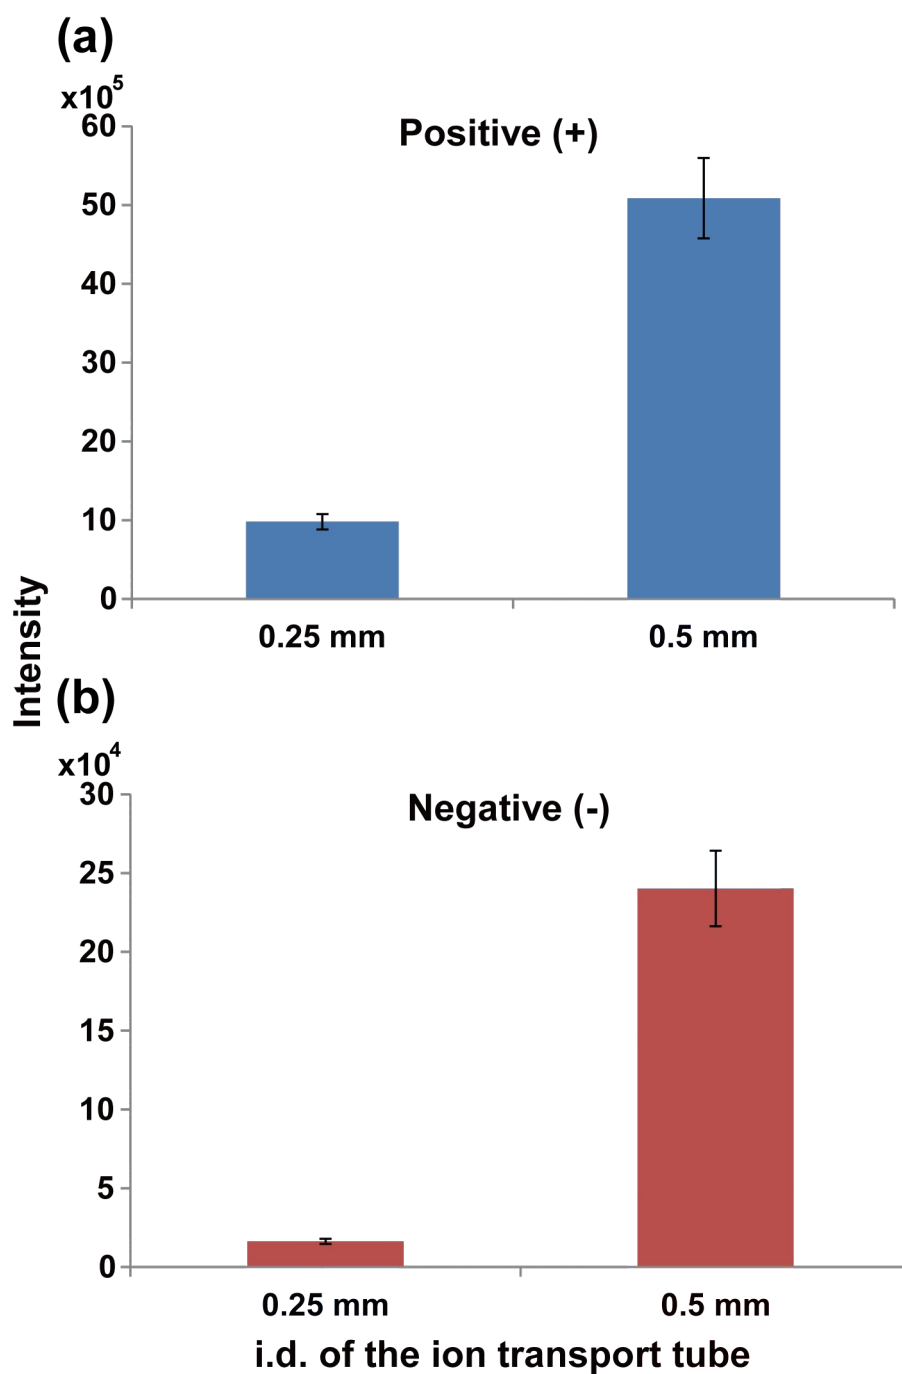

Supplementary Figure S1. Ion intensities for cytochrome c obtained with ion transmission tubes with different inner diameters (0.25 mm and 0.5 mm) in **a)** positive, and **b)** negative modes. The ion source pressures for both cases were optimized at around 2 bar.