

Electronic Supplementary Information

A sensitive one-step method for quantitative detection of α -amylase in serum and urine using personal glucose meter

Qing Wang, Hui Wang, Xiaohai Yang,* Kemin Wang,* Rongjuan Liu, Qing Li and Jinqing Ou
*State Key Laboratory of Chemo/Biosensing and Chemometrics, College of Chemistry and Chemical Engineering,
Key Laboratory for Bio-Nanotechnology and Molecular Engineering of Hunan Province, Hunan University,
Changsha 410082, China*

E-mail: kmwang@hnu.edu.cn; yangxiaohai@hnu.edu.cn. Tel/Fax: +86 731 88821566.

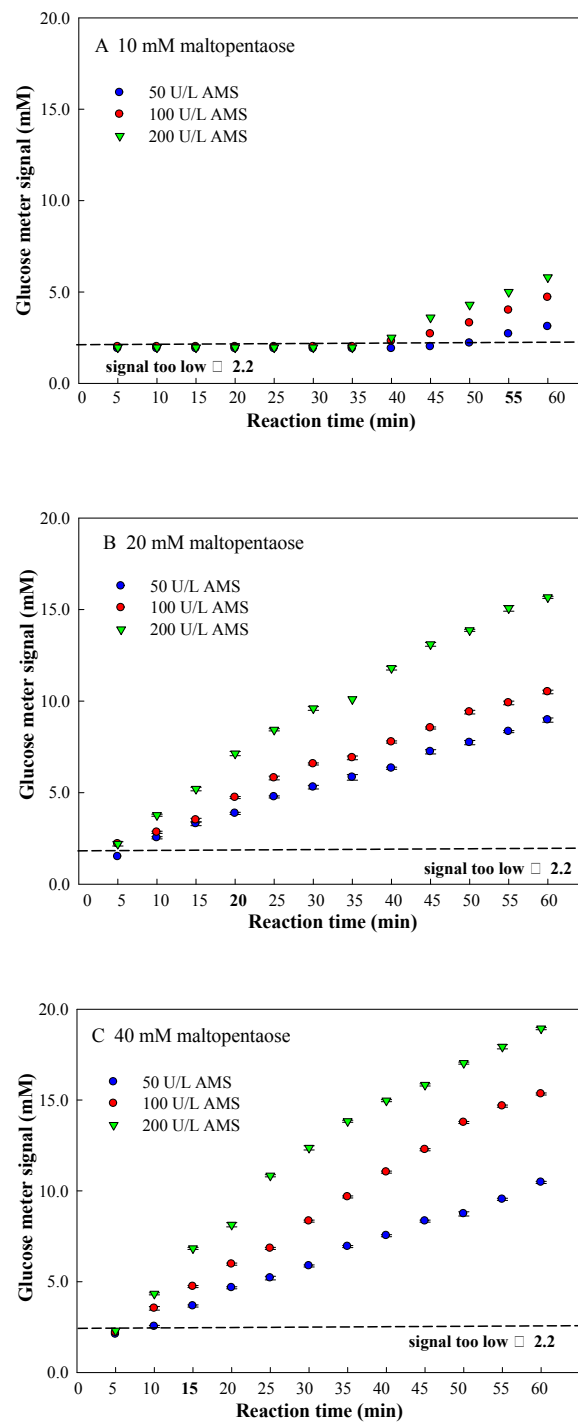


Fig. S1 The effect of maltopentaose concentration.

The incubation temperature was 37 °C. The error bars represent the standard deviation of three measurements. A signal of PGM larger than 2.2 mM was regarded as signal.