

SUPPORTING INFORMATION

For

Amplified detection of bleomycin based on an electrochemically driven recycling strategy

Shan Lu,^a Mei Yang,^b Xiaoxi Li,^c Xinjian Liu,^c Yongmei Yin,^{a*} and Ya Cao^{b*}

^a Department of Oncology, the First Affiliated Hospital of Nanjing Medical University, Nanjing 210029, China.

^b Laboratory of Biosensing Technology, School of Life Sciences, Shanghai University, Shanghai 200444, China.

^c State Key Laboratory of Pharmaceutical Biotechnology, Department of Biochemistry, Nanjing University, Nanjing 210093, China.

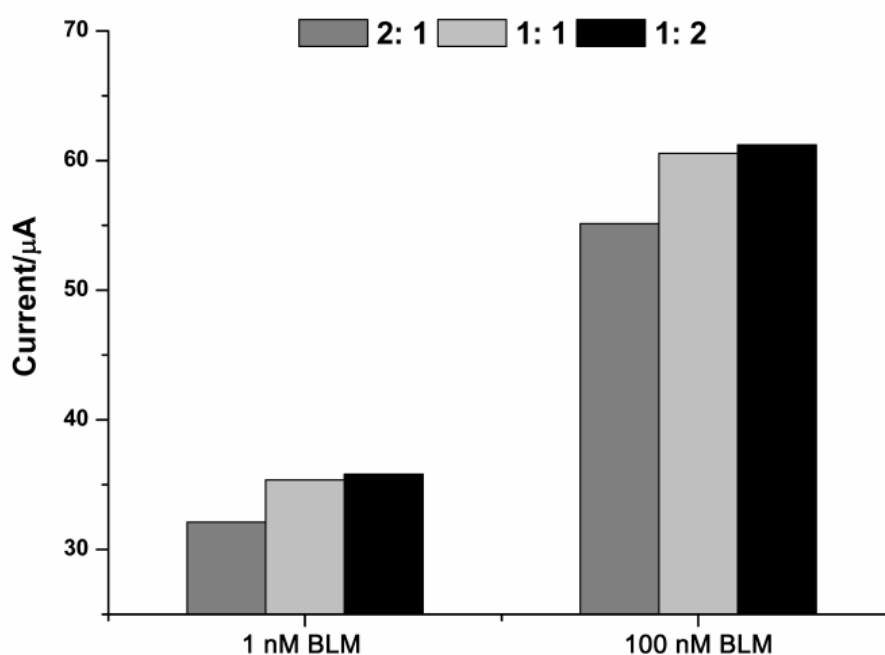


Fig. S1 Effect of molar ratio of BLM and Fe²⁺ on DPV peak currents.