

Method Development Report

MS1 Resolution	0.75
MS2 Resolution	0.75
Calibration Method	C:\MassLynx\IntelliStart\Results\Unit Mass Resolution\Calibration_20141016_2.cal
Tune Method	C:\Massdata2014\MHBMA.PRO\ACQUDB\MHBMA .IPR
Cone Voltage Range	2 - 100
Collision Energy Range	2 - 80
Lowest Fragment Mass	80.00
Excluded Losses	18.00, 44.00

Date: Generated on Wed 04 Mar 2015 at 16:52

Results

IntelliStart generated the following experiments:

MRM Experiment	C:\Massdata2014\MHBMA.PRO\ACQUDB\D7-DHBMA-15-03-04.exp
----------------	--



IntelliStart found the following compounds:

Compound	Formula/Mass		Parent m/z	Cone Voltage	Daughters	Collision Energy	Ion Mode
D7-DHBMA	258	1	257.03	26	128.05	14	ES-
		2	257.03	26	110.03	22	ES-

Compound



D7-DHBMA
(258)



Transition 1: ES-, m/z 257.03 → 128.05

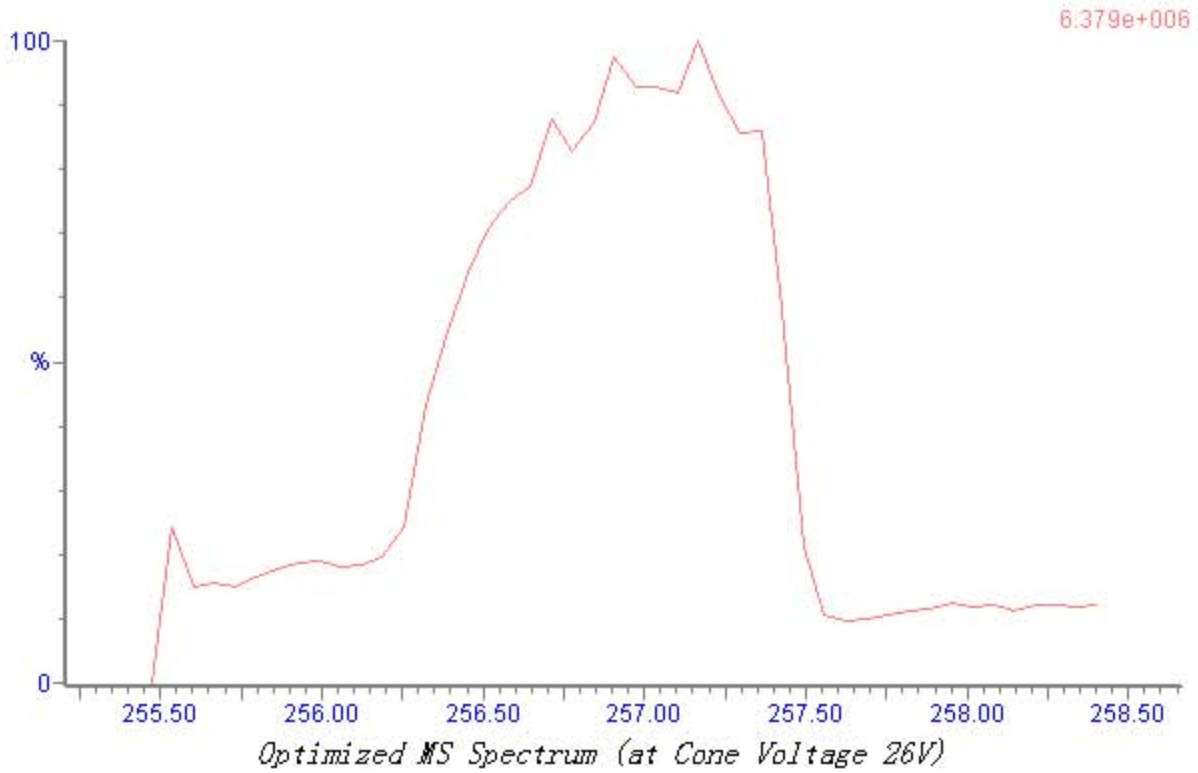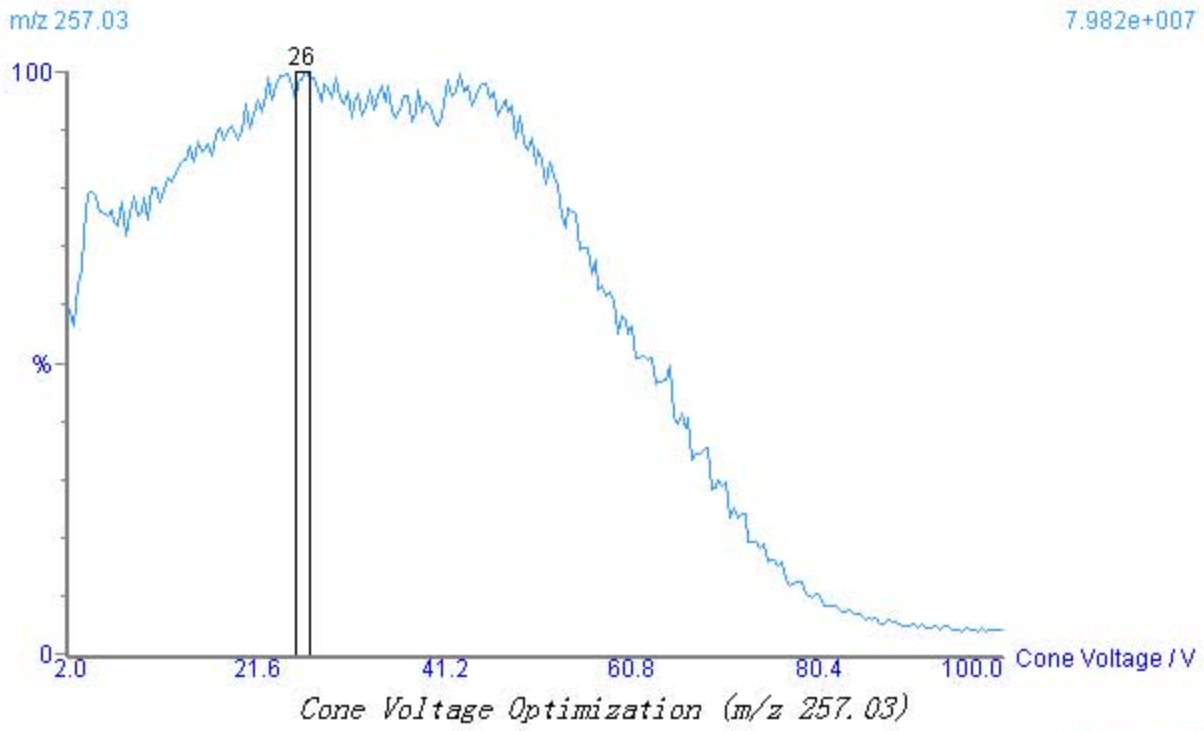

m/z 257.03 -> 128.05


2.274e+007

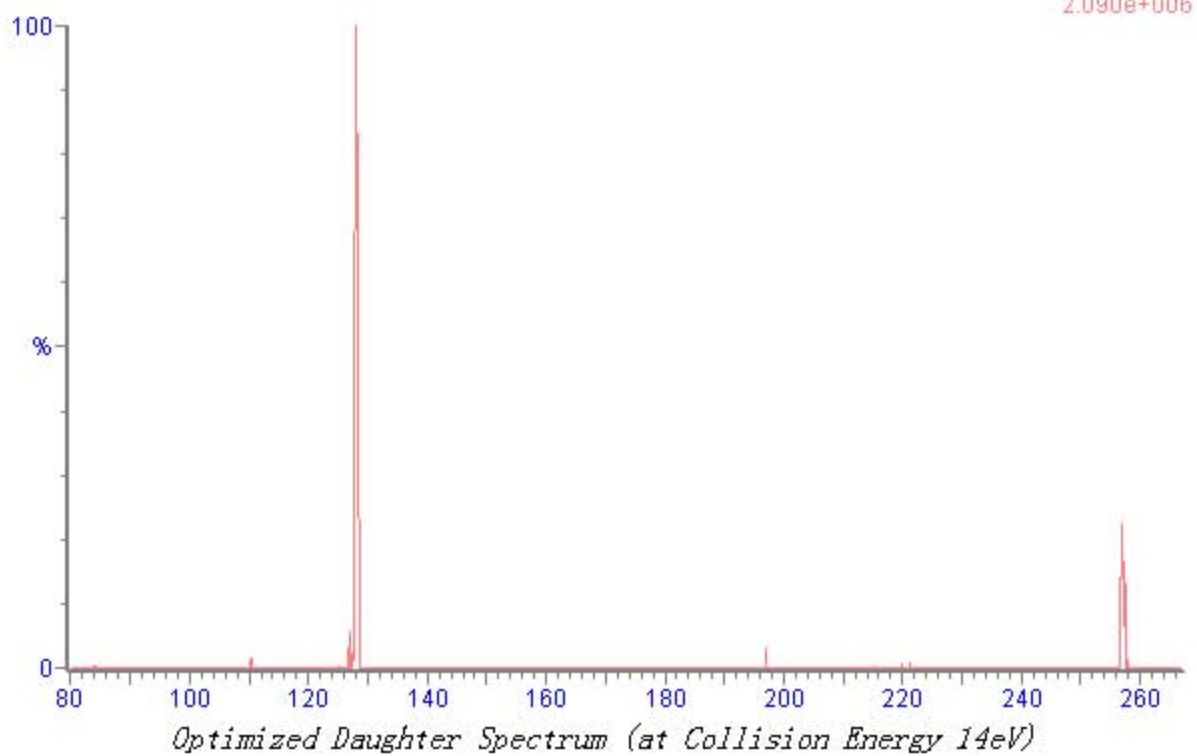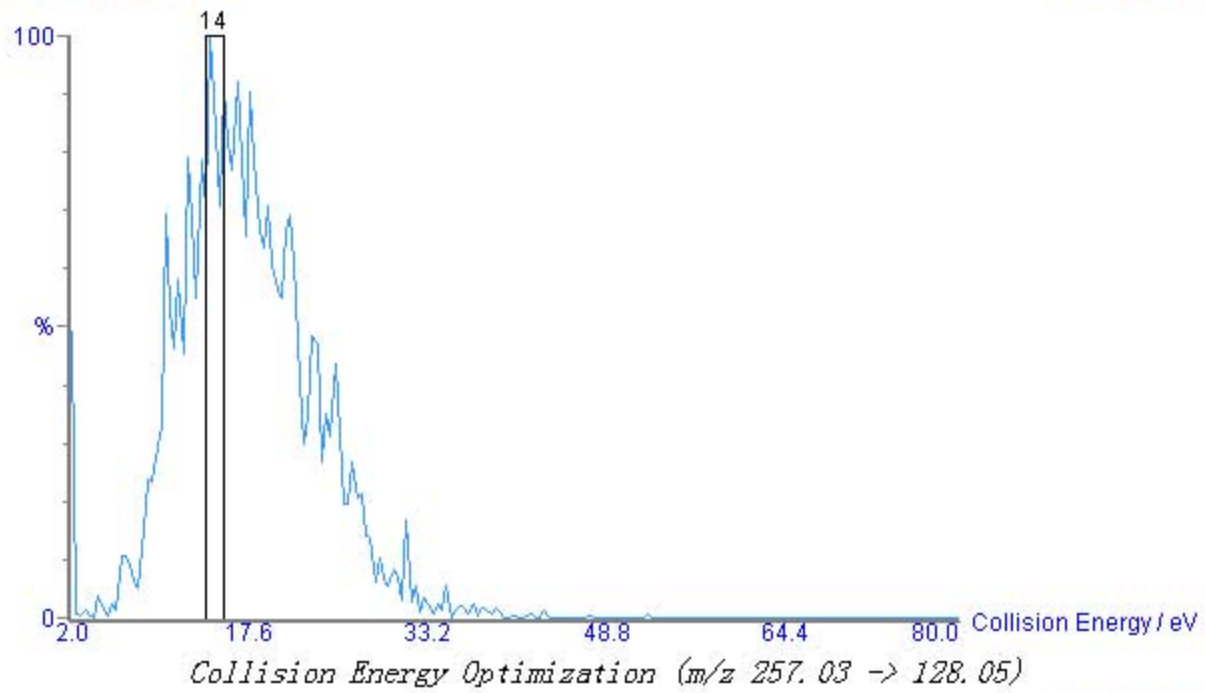**Transition 2: ES-, m/z 257.03 -> 110.03**

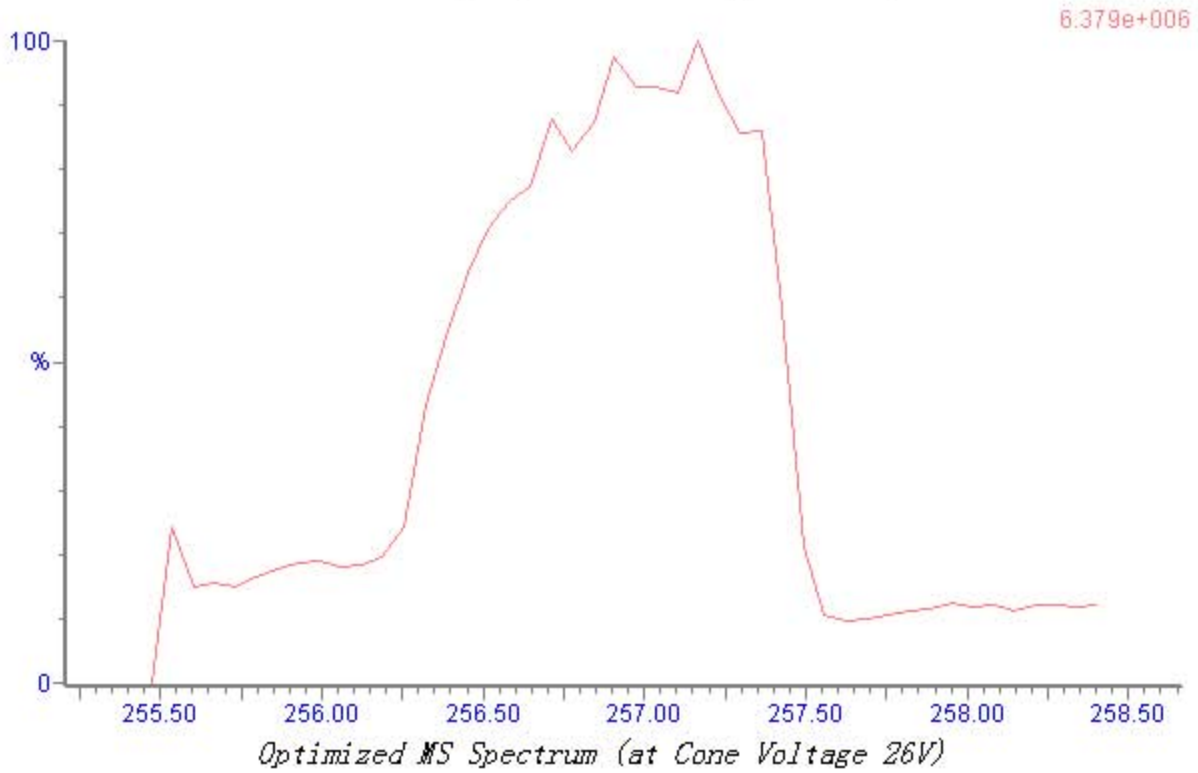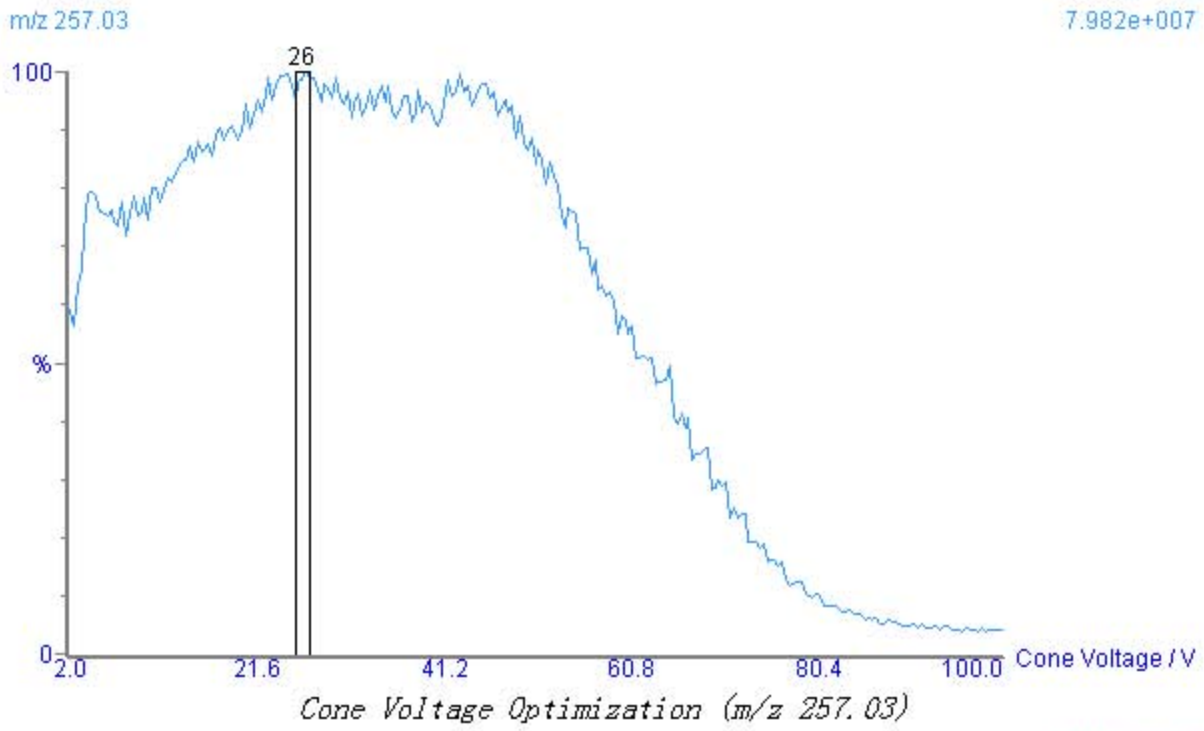

m/z 257.03 -> 110.03

9.226e+005

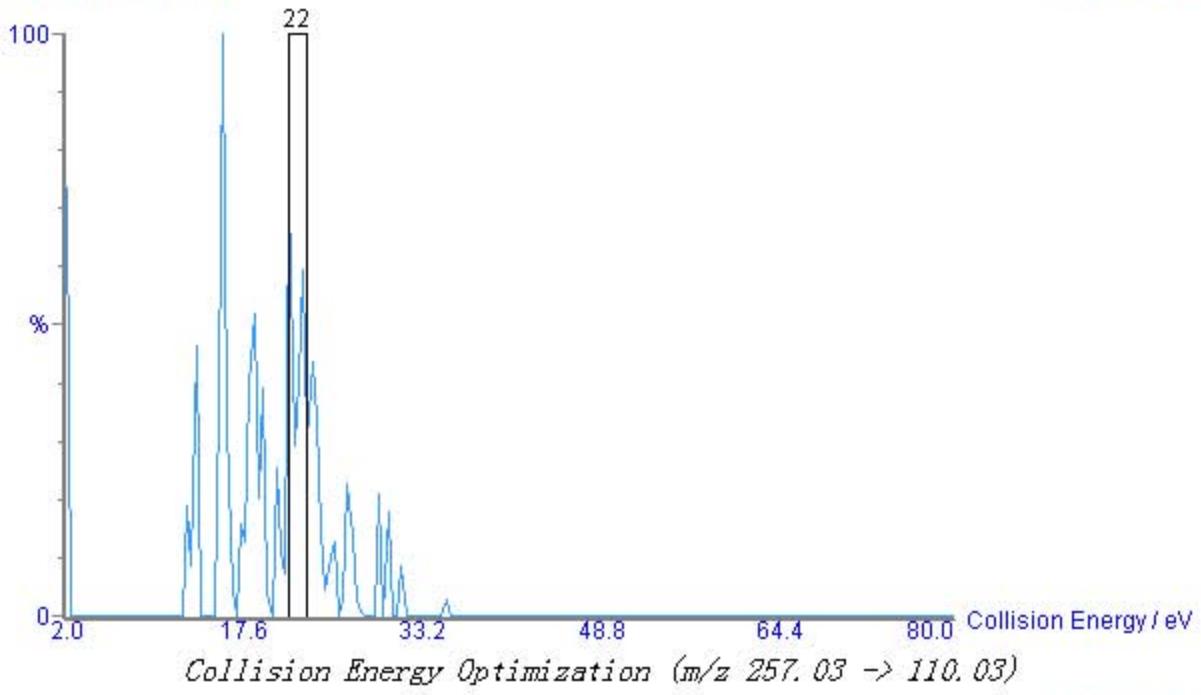

9.553e+005

