

Electronic Appendix 3

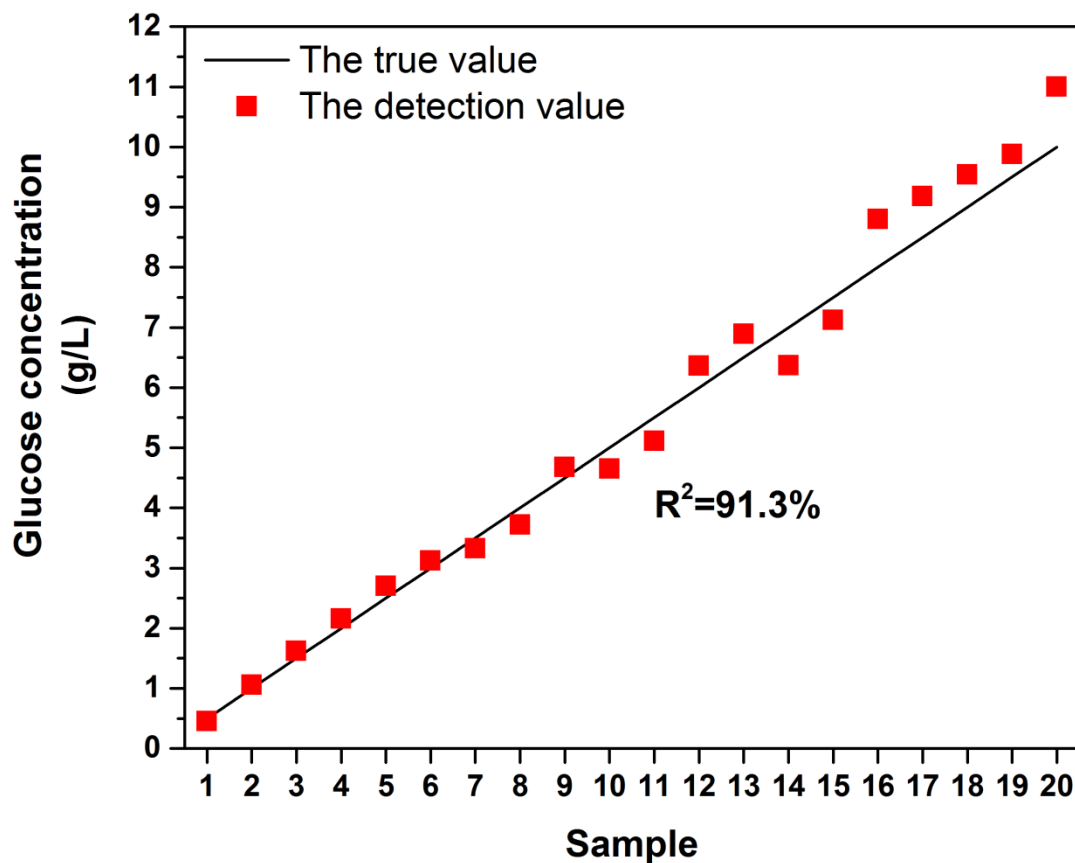


Figure S1: The accuracy validation experiments for nonlinear fitting algorithm for glucose detection. The detection results and the true concentrations of 20 samples were used for comparison.