
Supplementary Information

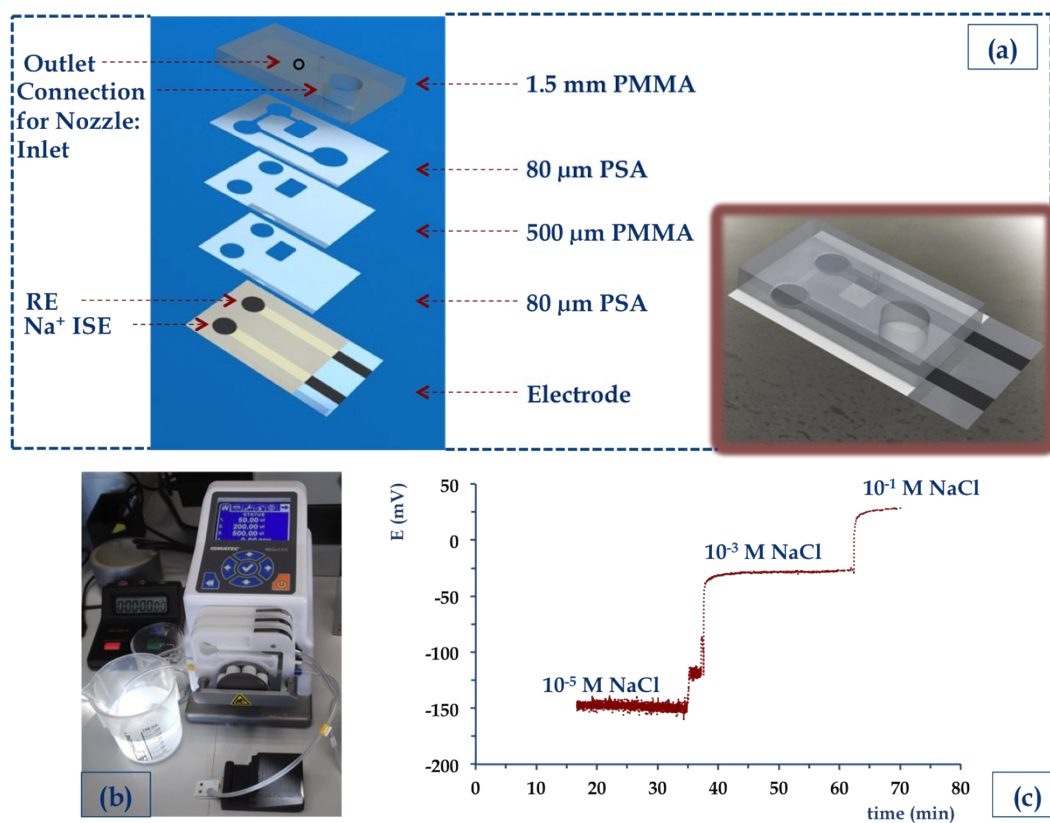


Figure SID. 1: (a) 1st generation of the Microfluidic unit integrated on top of the screen-printed electrodes and (b) the experimental set-up used to carry out the first on-bench tests (i.e. potentiometric strip connected to a peristaltic pump). (c) Example of a three-point calibration curve realised using the set-up in (b).

Figure SID. 2: Views of the wearable PotMicroChip worn on the upper arm

