

### Capability of fs-LA-ICP-MS for sulfide analysis in comparison to ns-LA-ICP-MS: Reduction of laser induced matrix effects?

Cora C. Wohlgemuth-Ueberwasser and Klaus Peter Jochum

Electronic Supplementary Information

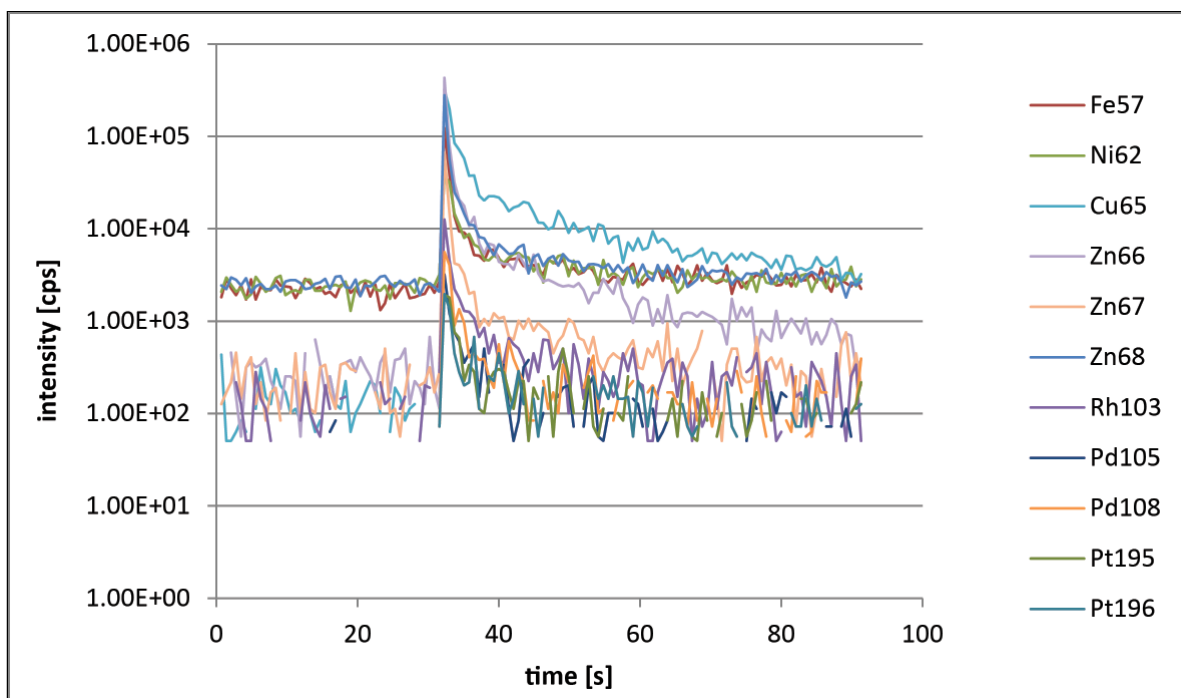


Figure S1