

Supporting Information

Ms. No. LC-ART-09-2015-001136

November 27, 2015

**An Exothermic Chip for Point-of-Care Testing Using a Forehead
Thermometer as Readout**

Bingbing Gao, Hong Liu,* and Zhongze Gu*

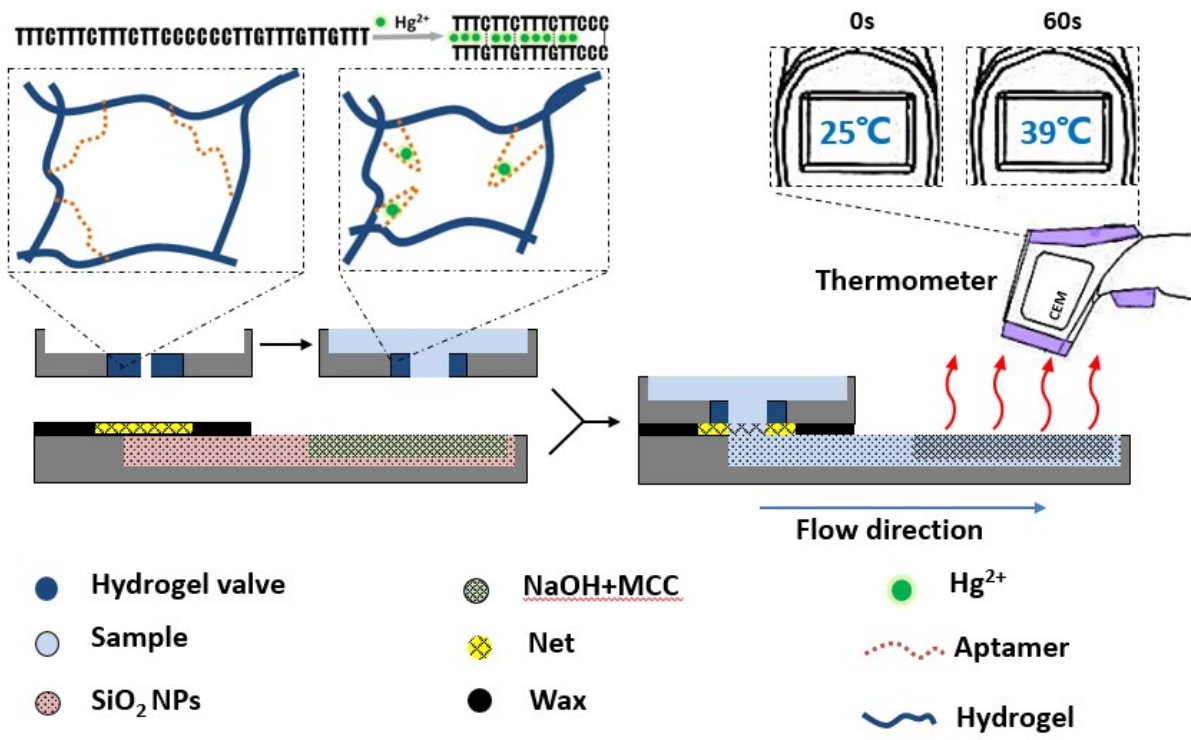


Figure S1. Schematic illustration of sampling part and euthermic part of the exothermic chip for Hg²⁺ detection. MCC: microcrystalline cellulose.