

Supplementary Information

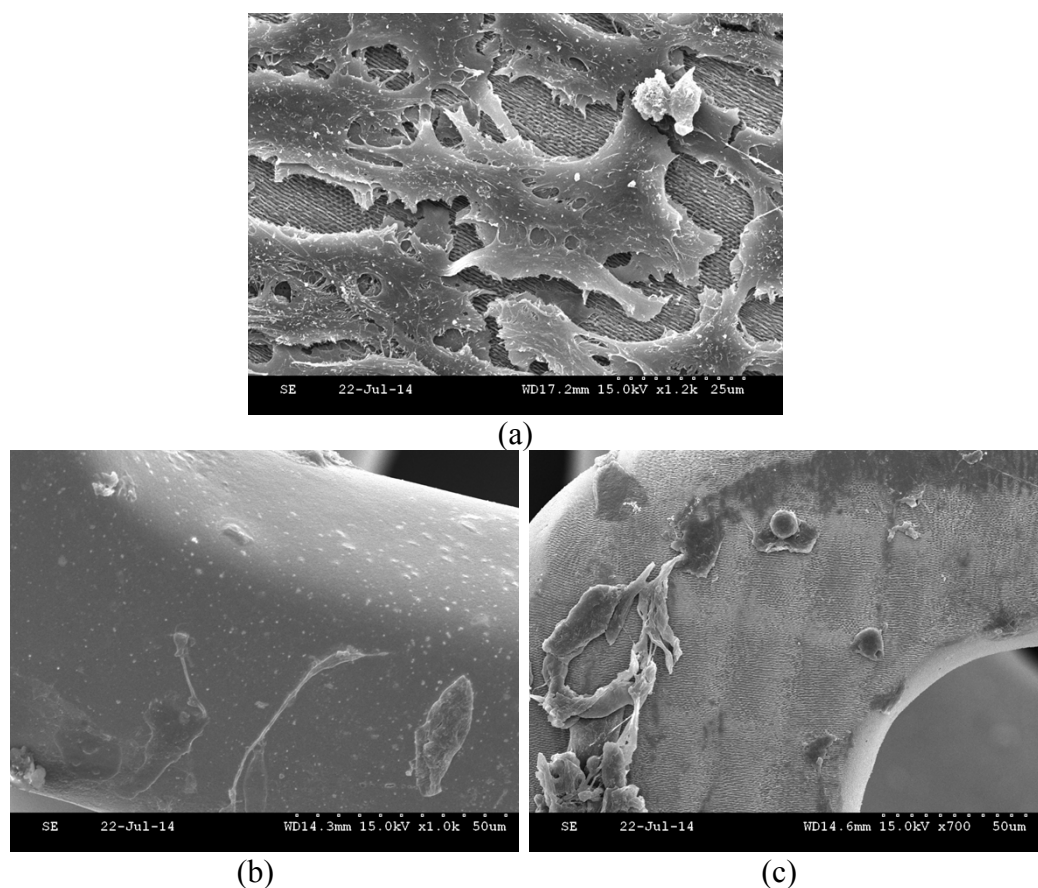


Fig A. HPMEC cells attached to (a) flat SS, (b) bare Pt:SS stent and (c) LIPSS covered Pt:SS stent generated at 1030 nm.