

Supporting Information for **Electrochemical Detection of Single Micelles through ‘Nano-Impacts’**

By Her Shuang Toh¹, and Richard G. Compton^{1*}

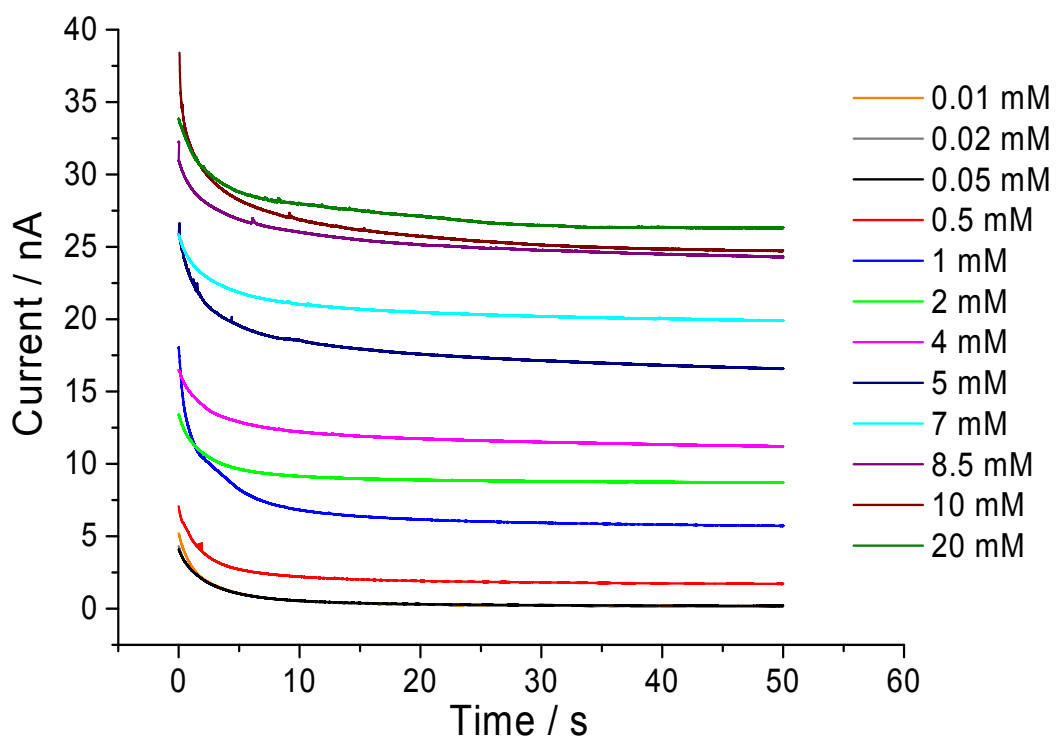


Figure S1. The chronoamperograms performed on solutions with 0.1 M sodium nitrate and different CTAB concentrations.

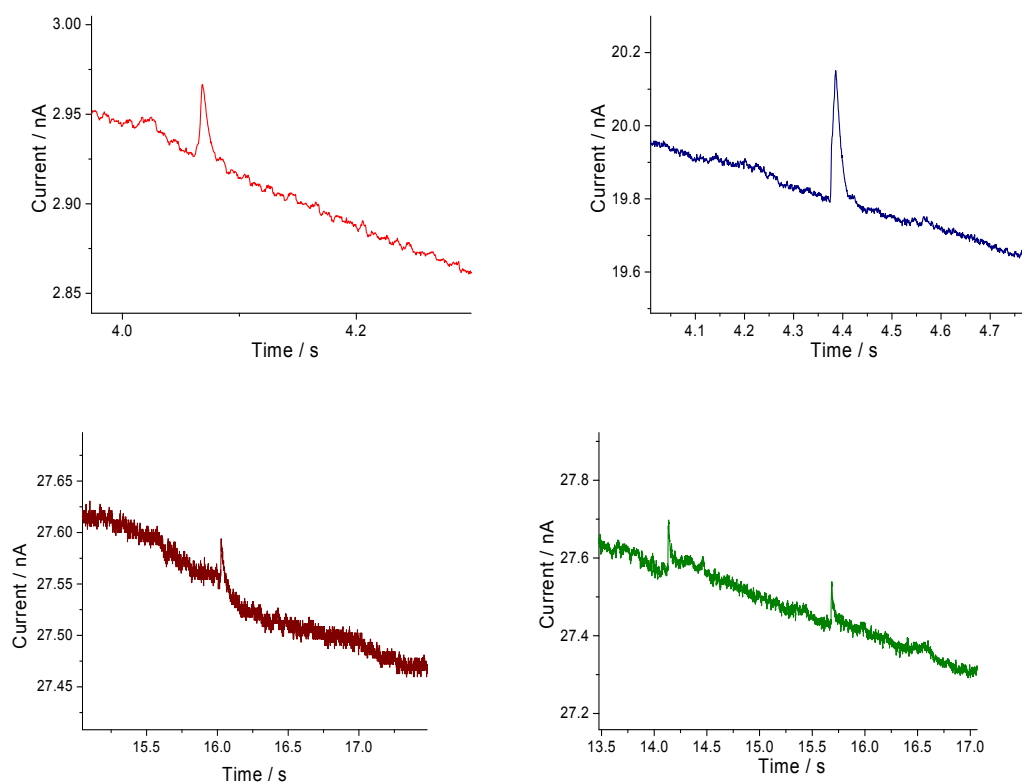


Figure S2. Examples of 'spikes' observed in the chronoamperogram at CTAB concentrations of A) 0.5 mM B) 5 mM C) 10 mM D) 20 mM.