

Fig. S1 Three dimensional diagram of the real sample, analysis of milk sample by direct injection at the flow rate of 1 mL min^{-1} (A), 1 mL min^{-1} (B).

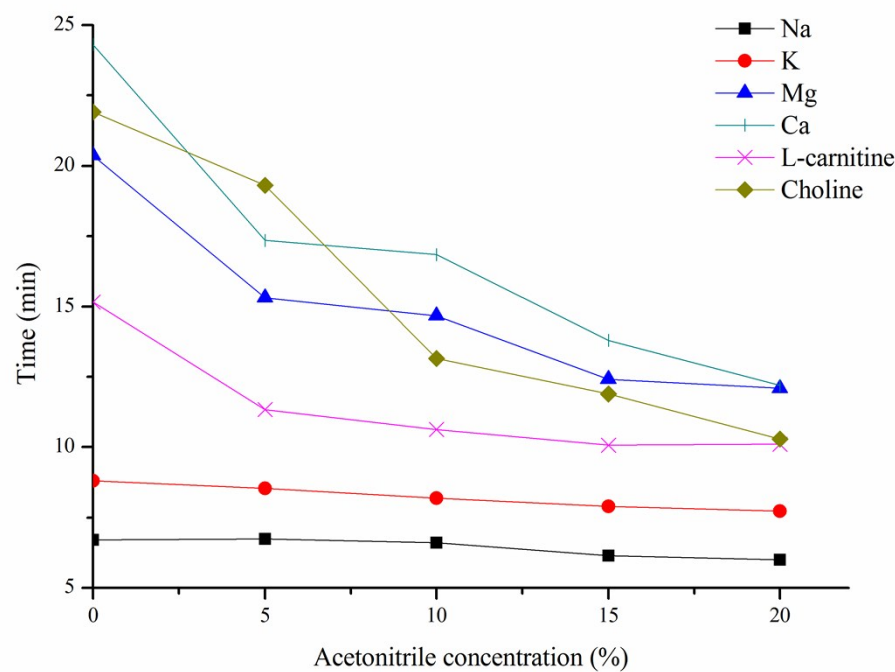


Fig. S2 The ratio of acetonitrile on the separation performance of analytical column