

A fluorescence-enhanced probe for rapid detection of formaldehyde and its application for cell imaging

Feng Wu,^{a,b} Yue Zhang,^b Lei Huang,^b Dan Xu,^{a,*} Hongying Wang^{b,*}

^a Clinical Medical College of Tianjin Medical University, Tianjin 300270, P.R. China.
E-mail: xudan8001@126.com (D. Xu)

^b School of Chemistry and Chemical Engineering, Tianjin University of Technology, Tianjin 300384, P.R. China. E-mail: hywang243@126.com (H. Wang)

Table of Contents

1. ¹H NMR, ¹³C NMR and HRMS spectra of **ANI**
2. The HRMS spectrum of **ANI** + **FA**

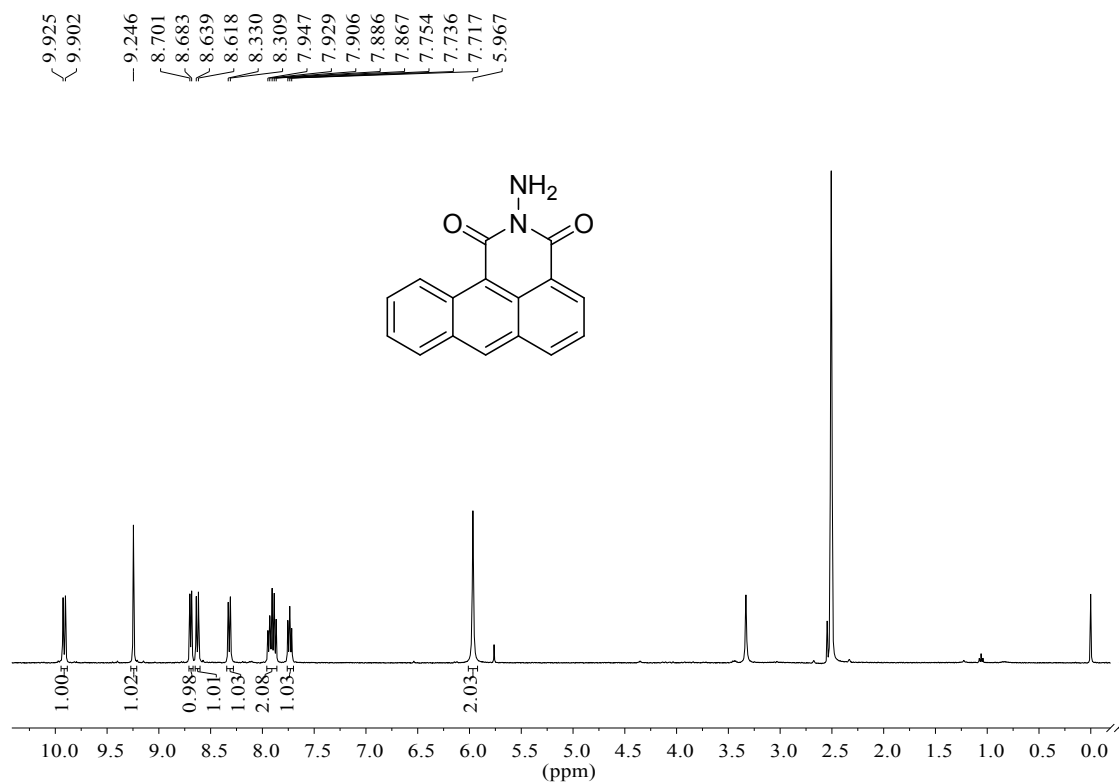


Figure S1. The ¹H NMR spectrum of ANI in DMSO-*d*₆ (400 MHz)

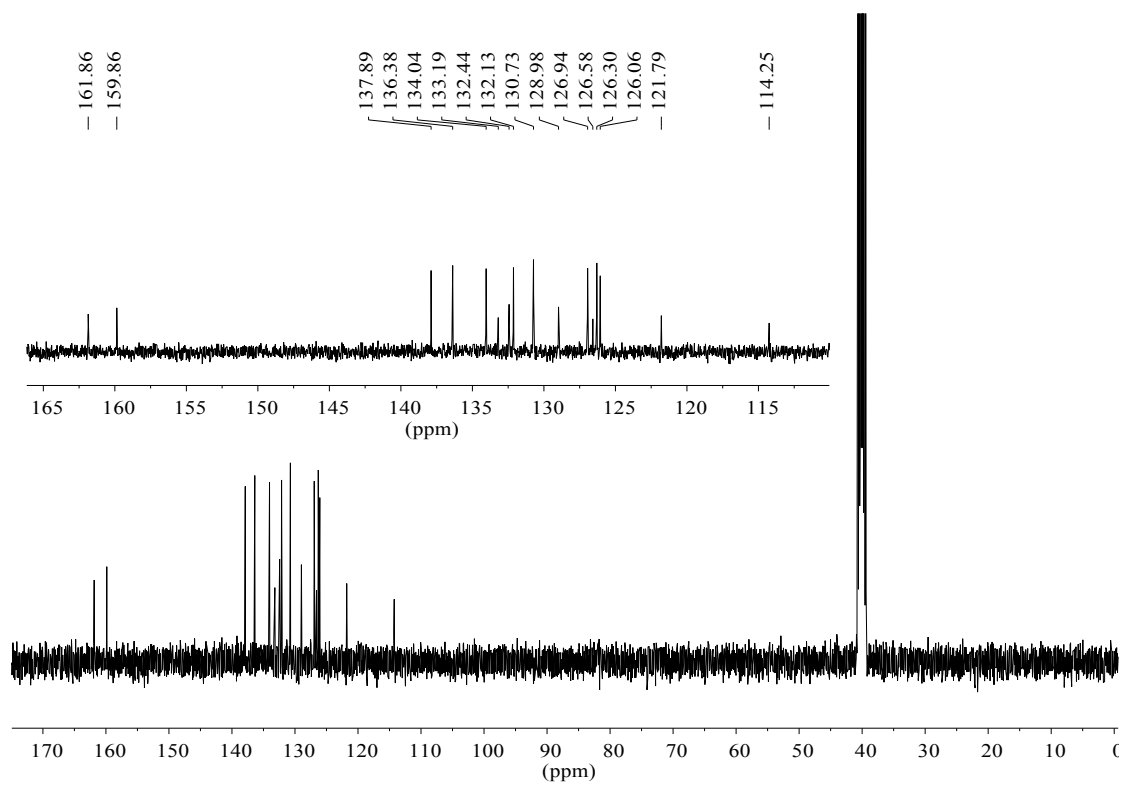


Figure S2. The ¹³C NMR spectrum of ANI in DMSO-*d*₆ (100 MHz)

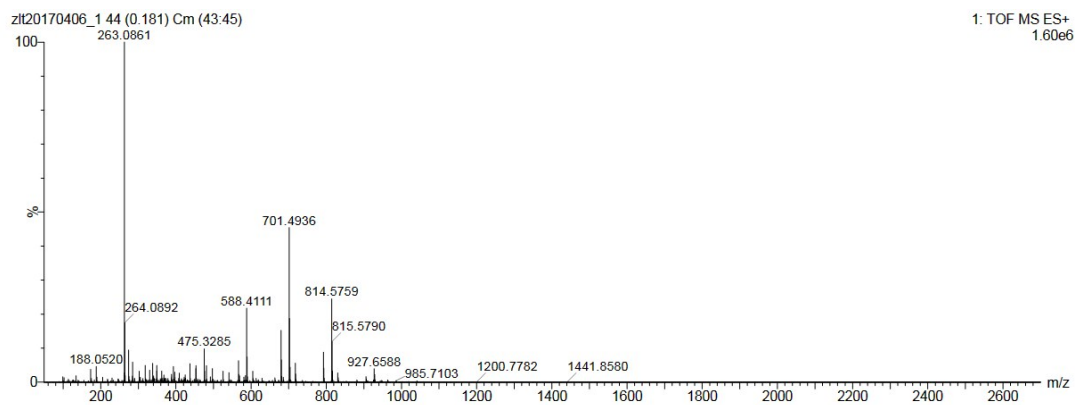


Figure S3. The HRMS spectrum of ANI

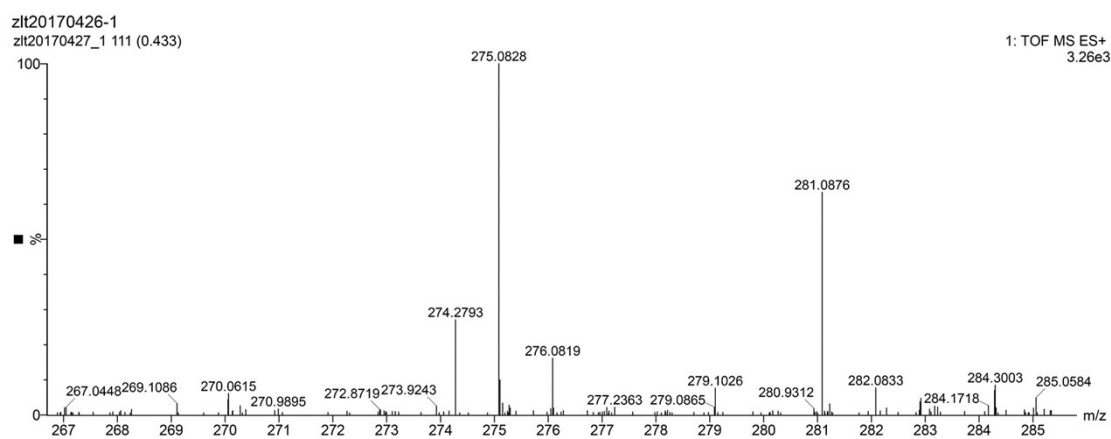


Figure S4. The HRMS spectrum of ANI + FA