


Qualitative Analysis Report

Data Filename	RL-1711-8.d	Sample Name	RL-1711-8
Sample Type	Sample	Position	Vial 41
Instrument Name	Agilent 6530 Accurate-Mass Q-TOF	User Name	
Acq Method	Direct Mass-2017.m	Acquired Time	17-Nov-17 10:05:46 PM
IRM Calibration Status	Success	DA Method	Direct Mass.m
Comment			
Sample Group	Info.		
Acquisition SW	6200 series TOF/6500 series		
Version	Q-TOF B.05.00 (B5042.1)		


User Chromatograms

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

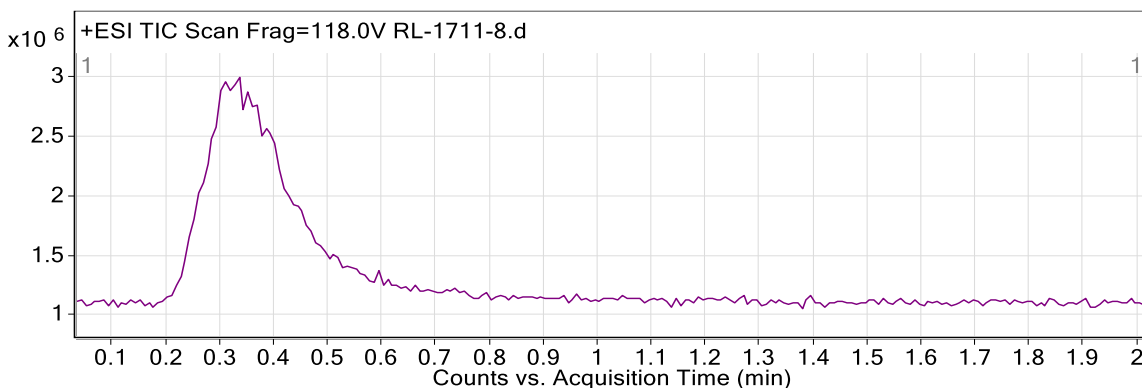

User Spectra

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

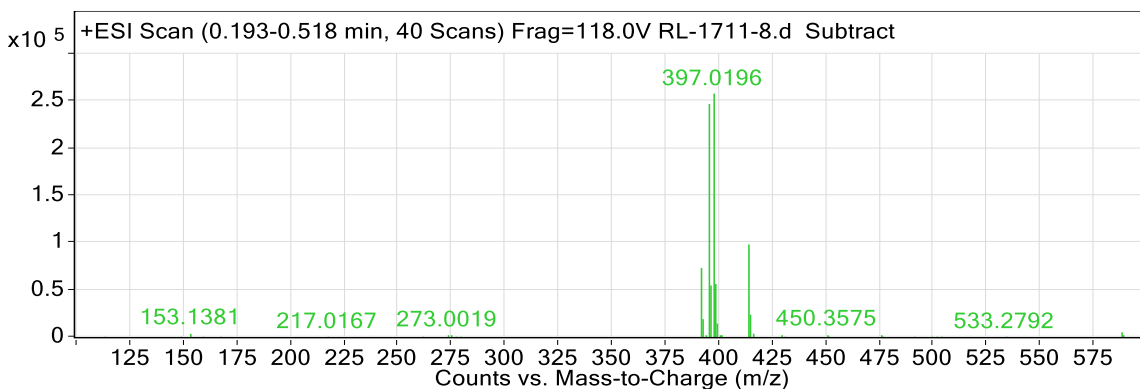



Peak List

m/z	z	Abund
391.2844	1	74972.84
392.2876	1	19376.4
395.0215	1	247987.09
396.0243	1	55762.69
397.0196	1	258735.02
398.0224	1	57005.21
399.0192	1	15645.87
413.2664	1	99096.18

Qualitative Analysis Report

414.2696	1	24863.98
803.5437	1	23517.95

Compounds

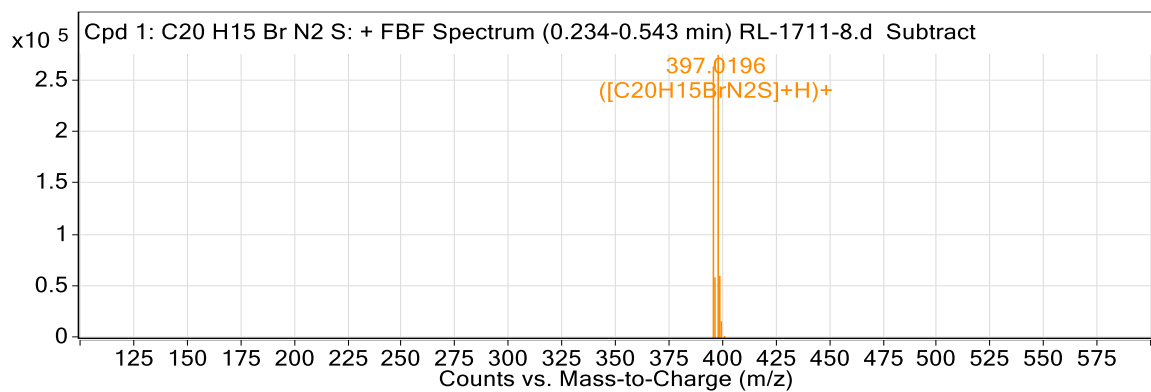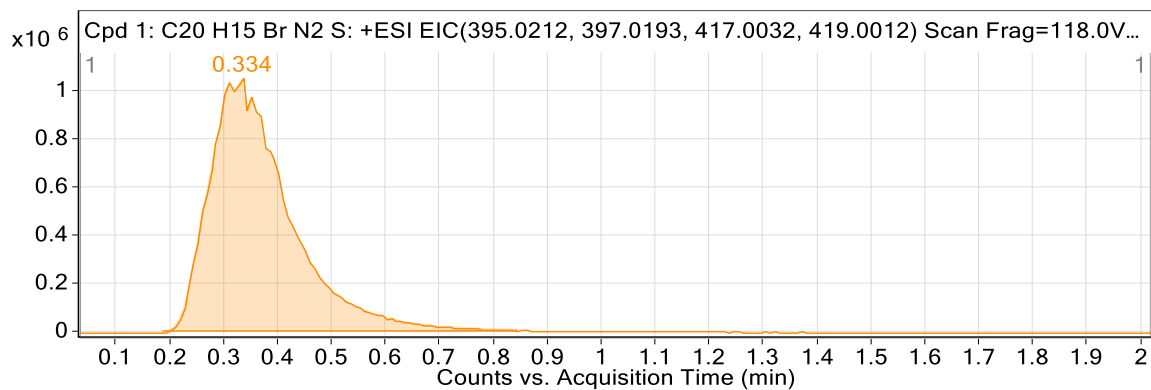

--- End Of Report ---