


Qualitative Analysis Report

Data Filename	RL-1M-6.d	Sample Name	RL-1M-6
Sample Type	Sample	Position	Vial 31
Instrument Name	Agilent 6530 Accurate-Mass Q-TOF	User Name	
Acq Method	Direct Mass-2017.m	Acquired Time	20-Nov-17 9:43:17 PM
IRM Calibration Status	Success	DA Method	Direct Mass.m
Comment			
Sample Group	Info.		
Acquisition SW	6200 series TOF/6500 series		
Version	Q-TOF B.05.00 (B5042.1)		


User Chromatograms

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

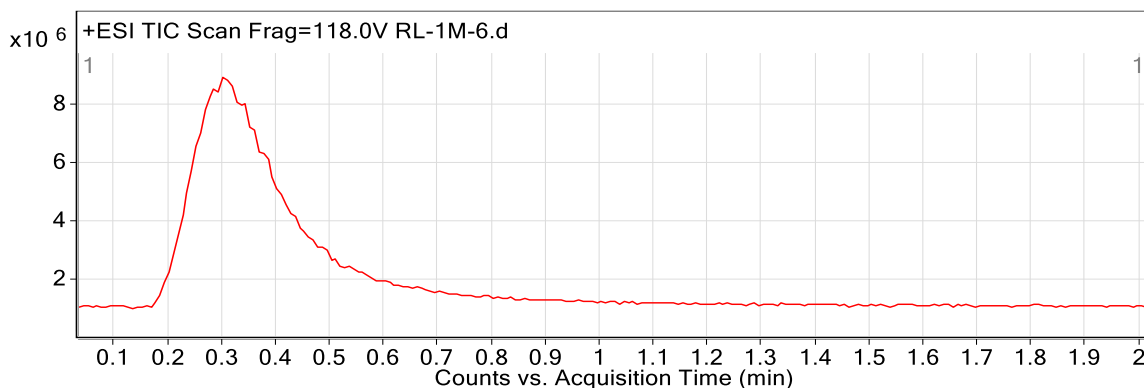

User Spectra

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

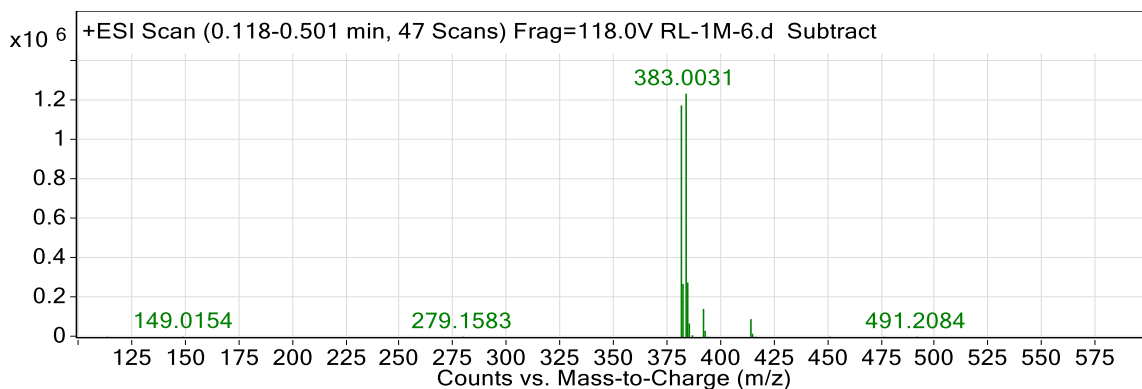



Peak List

m/z	z	Abund
381.0051	1	1176898
382.0083	1	271861.34
383.0031	1	1235625.38
384.0063	1	279430.81
385.0029	1	76875.88
391.2839	1	149720.36
392.2871	1	38262.59
413.2658	1	97007.55

Qualitative Analysis Report

414.269	1	24125.2
803.5427	1	41722.53

Compounds

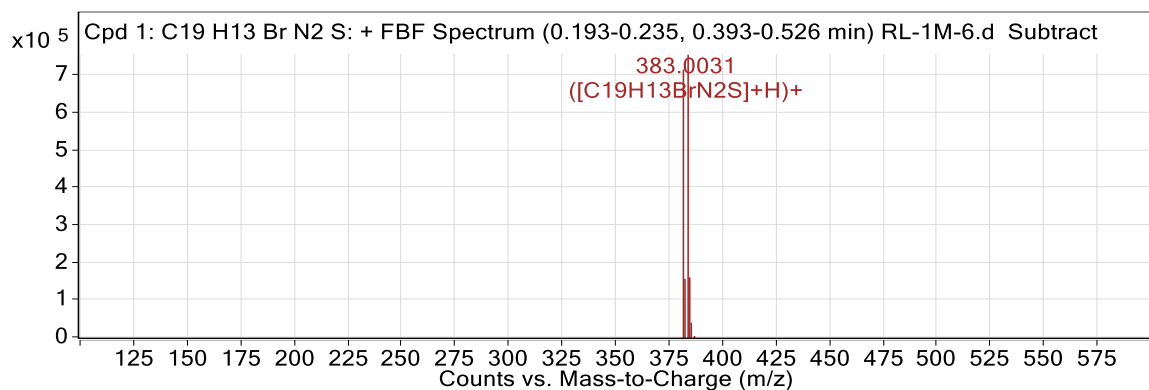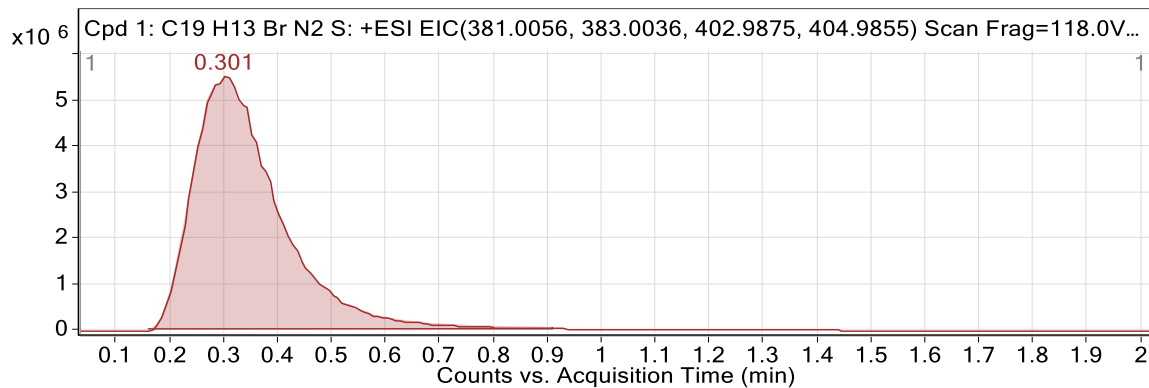

--- End Of Report ---