


Qualitative Analysis Report

Data Filename	RL-1811P-3.d	Sample Name	RL-1811P-3
Sample Type	Sample	Position	Vial 11
Instrument Name	Agilent 6530 Accurate-Mass Q-TOF	User Name	
Acq Method	Direct Mass-2017.m	Acquired Time	18-Nov-17 9:58:50 PM
IRM Calibration Status	Success	DA Method	Direct Mass.m
Comment			

Sample Group	Info.
Acquisition SW	6200 series TOF/6500 series
Version	Q-TOF B.05.00 (B5042.1)


User Chromatograms

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

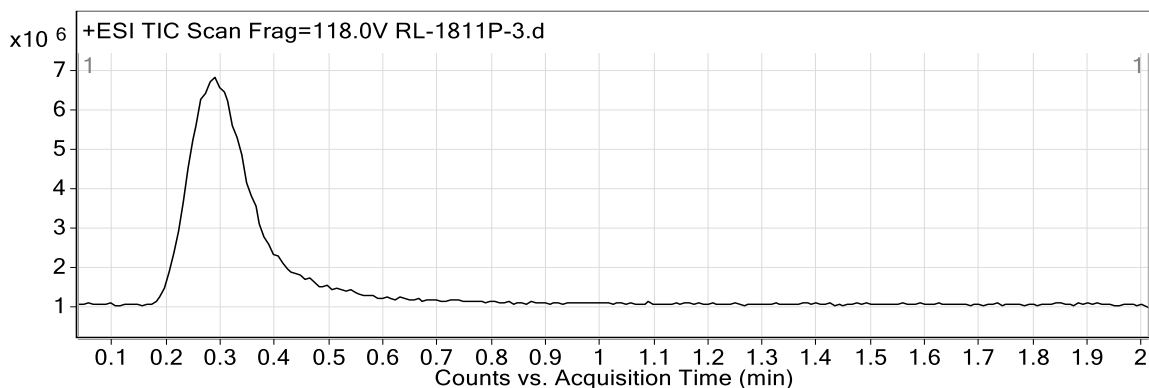

User Spectra

Fragmentor Voltage 118 Collision Energy 0 Ionization Mode ESI

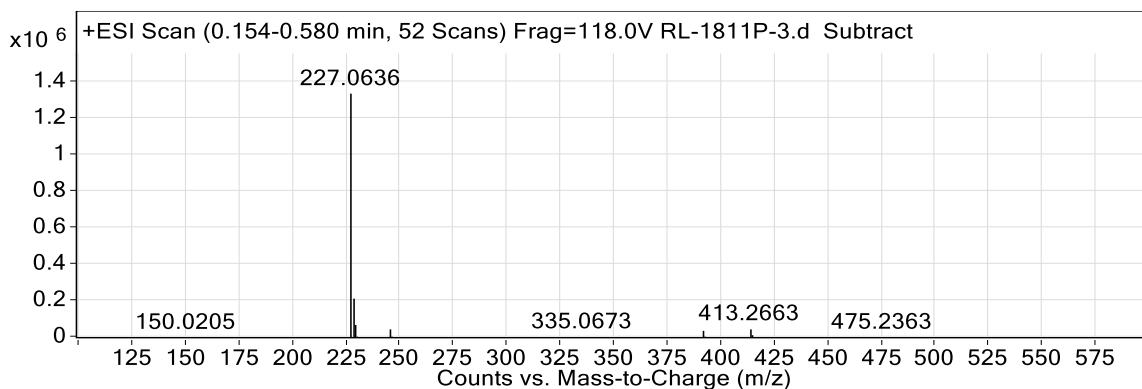



Peak List

m/z	z	Abund
227.0636	1	1336574.63
227.2007		45916.92
228.0667	1	218725.14
229.0617	1	71727.85
230.0631	1	9395.13
244.9568	1	49100.3
391.2843	1	42995.73
392.2878	1	11286.09

Qualitative Analysis Report

413.2663	1	48026.02
414.2695	1	12186.33

Compounds

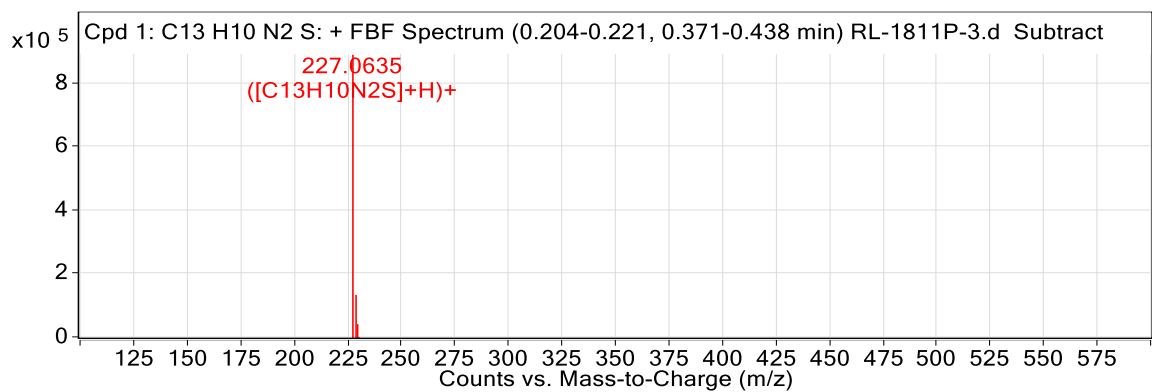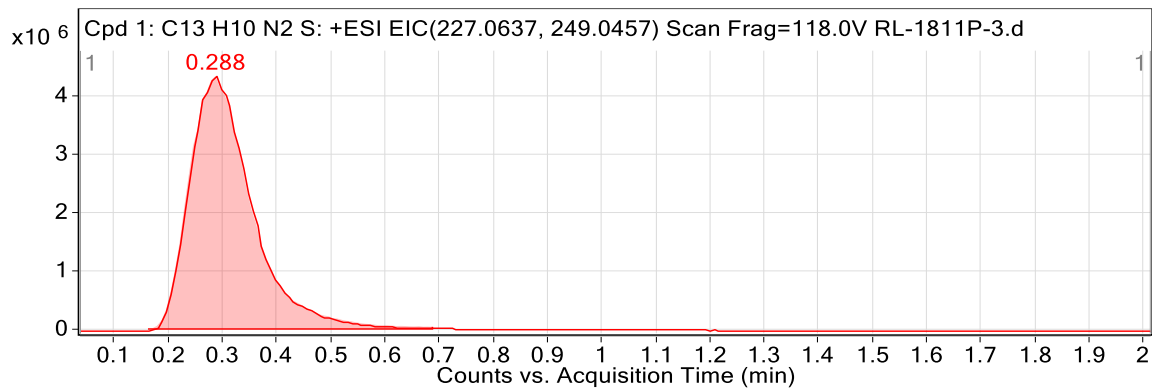

--- End Of Report ---