


Supplementary Figure caption


Supplementary Fig. S1. The mean SD result performed on HT-FTIR spectra of CT-DNA with different pretreatment temperature

Supplementary Fig. S2. The SNR result performed on HT-FTIR spectra of CT-DNA with different sample amounts

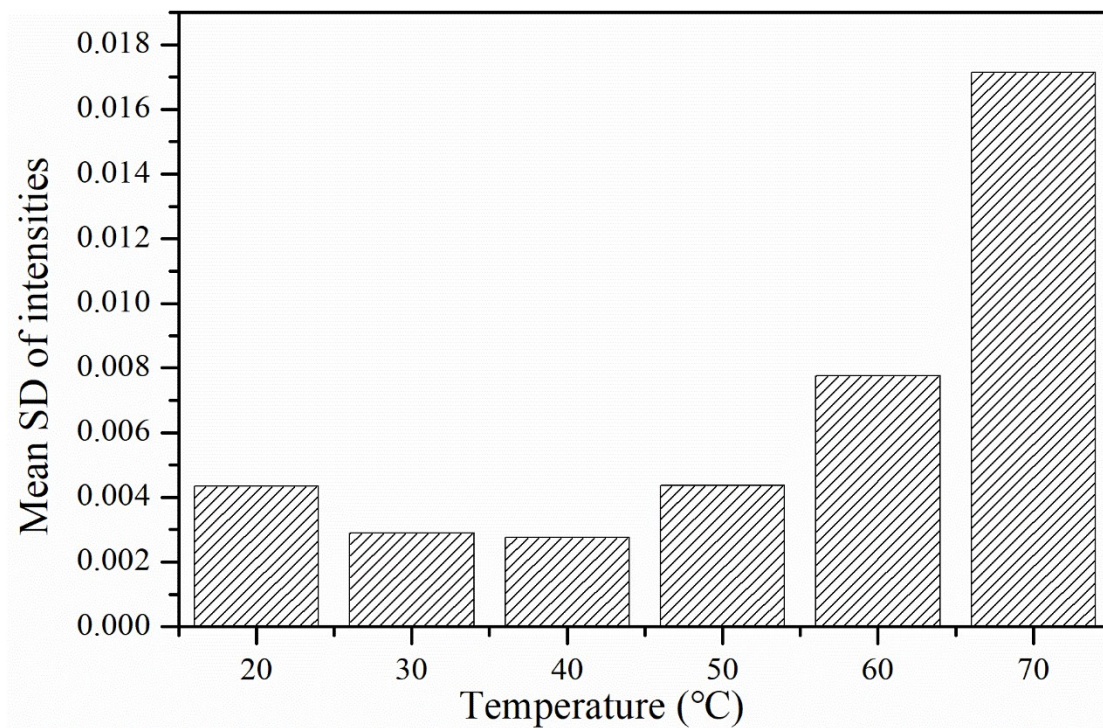

Note: SD refers standard deviation

Supplementary Fig. S1

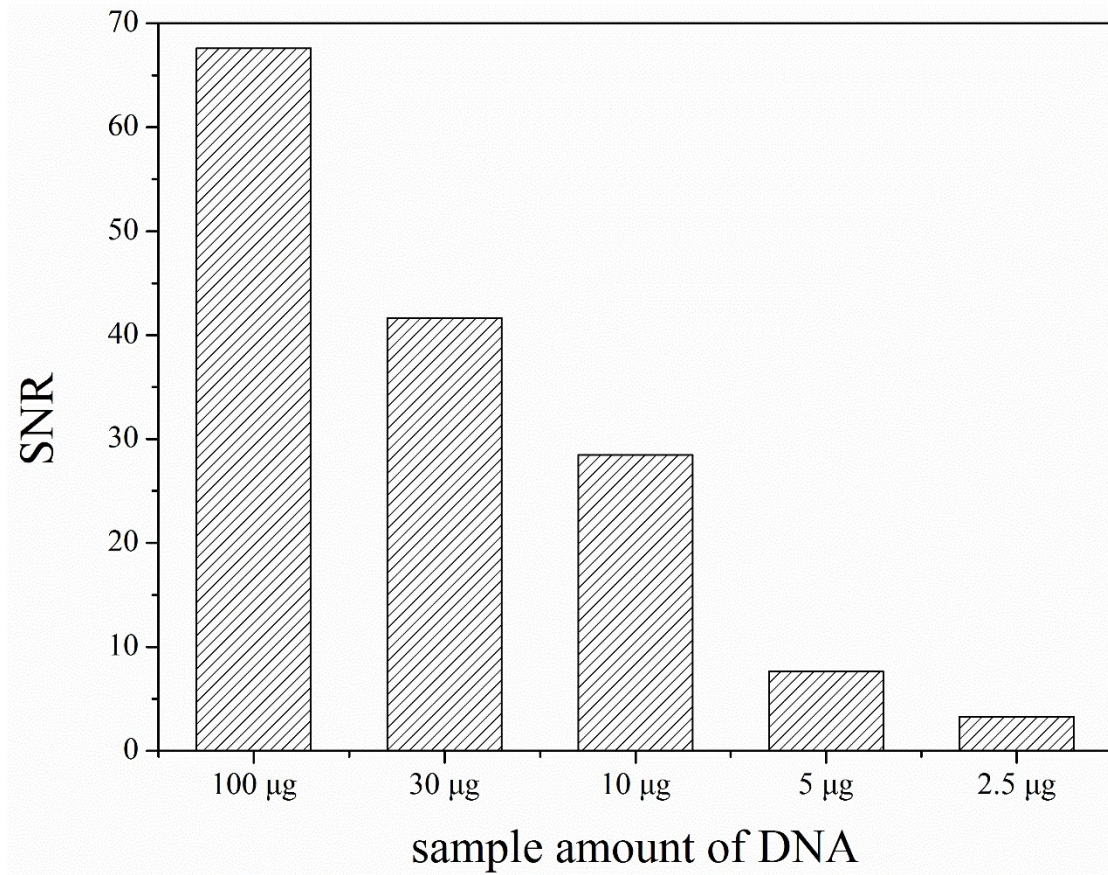

Note: SNR refers signal to noise ratio.

Supplementary Fig. S2