

Supplementary information for  
Chromatographic paper-based analytical devices using an  
oxidized paper substrate  
Yuki Hashimoto and Takashi Kaneta

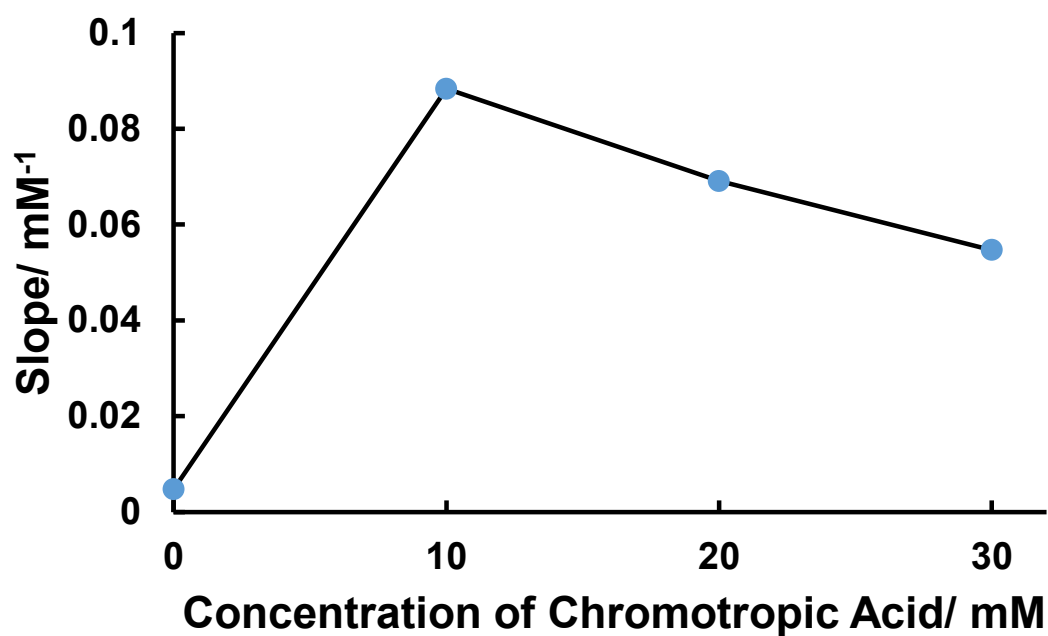


Fig. S1 Effect of the concentration of chromotropic acid on sensitivity. The sensitivity is expressed by the slope of calibration curves.