



## Supplementary Information


### Strain challenge

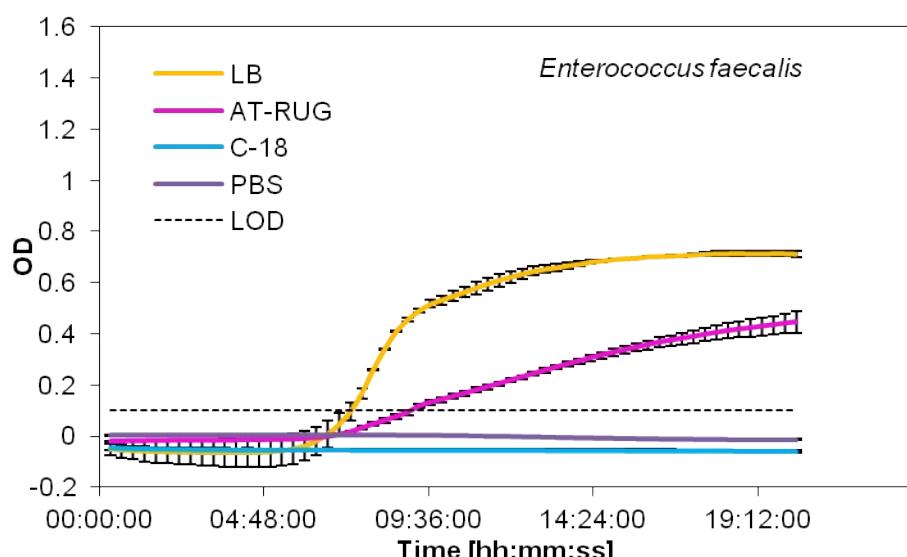


**Fig. S1** Growth curve of *Enterococcus faecalis* in different media measured at 365 nm.

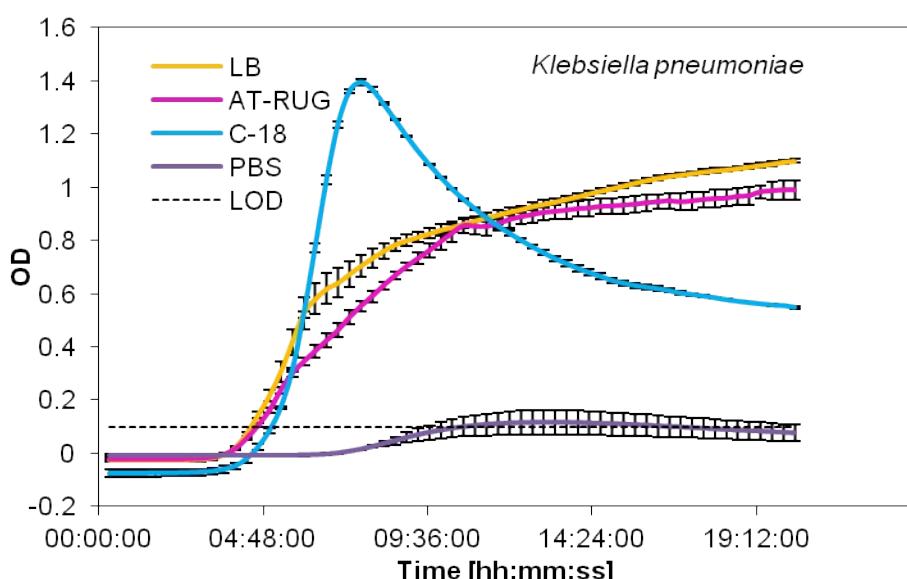


**Fig. S2** Growth curve of *Klebsiella pneumoniae* in different media measured at 365 nm.

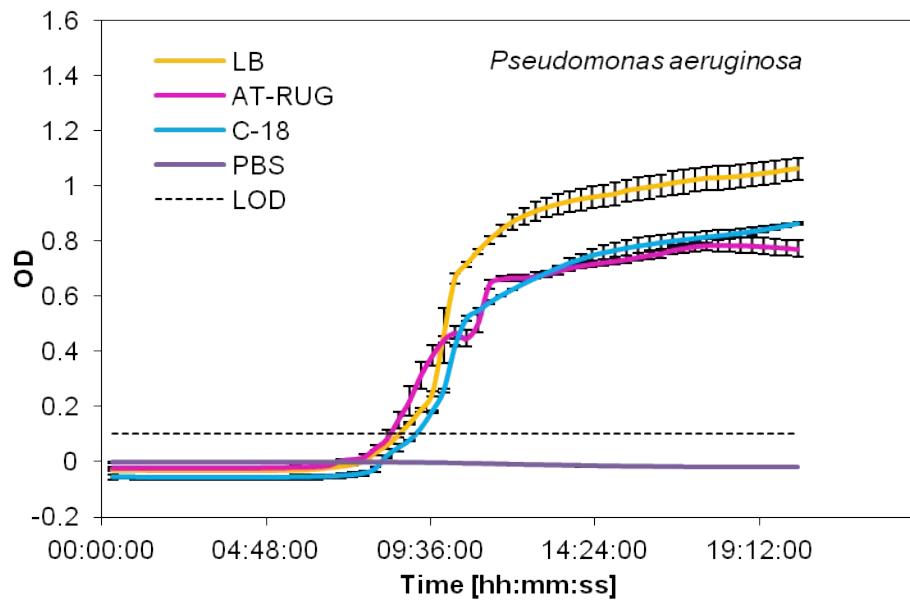


**Fig. S3** Growth curve of *Pseudomonas aeruginosa* in different media measured at 365 nm.

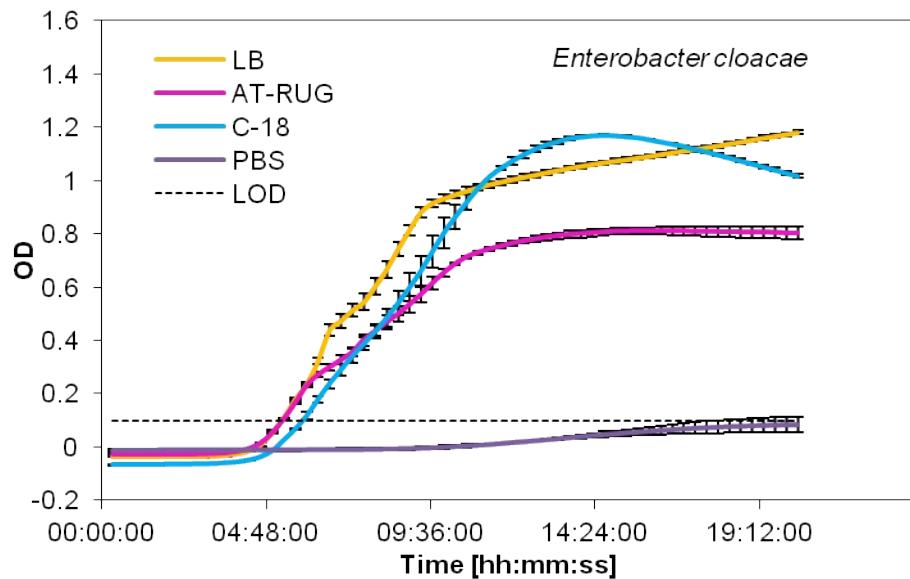


**Fig. S4** Growth curve of *Enterobacter cloacae* in different media measured at 365 nm.

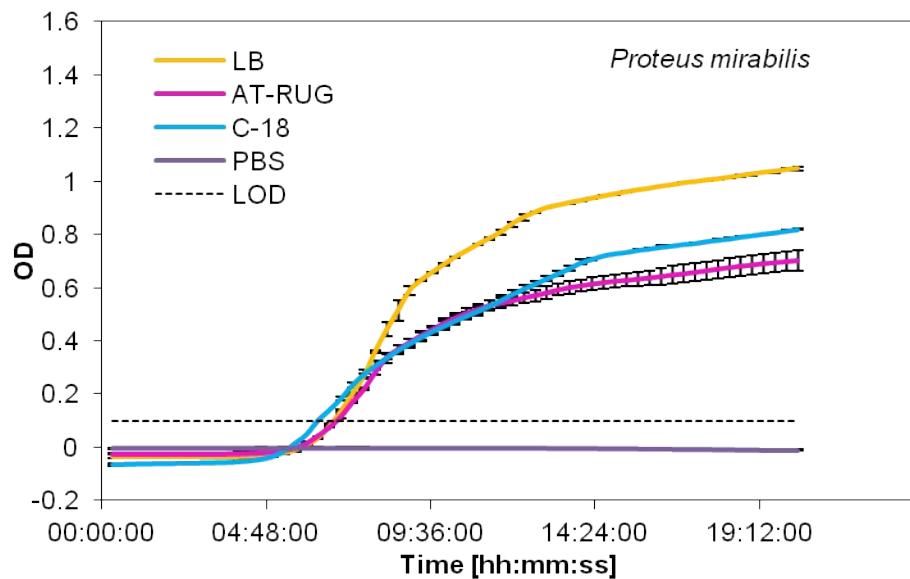

**Fig. S5** Growth curve of *Proteus mirabilis* in different media measured at 365 nm.

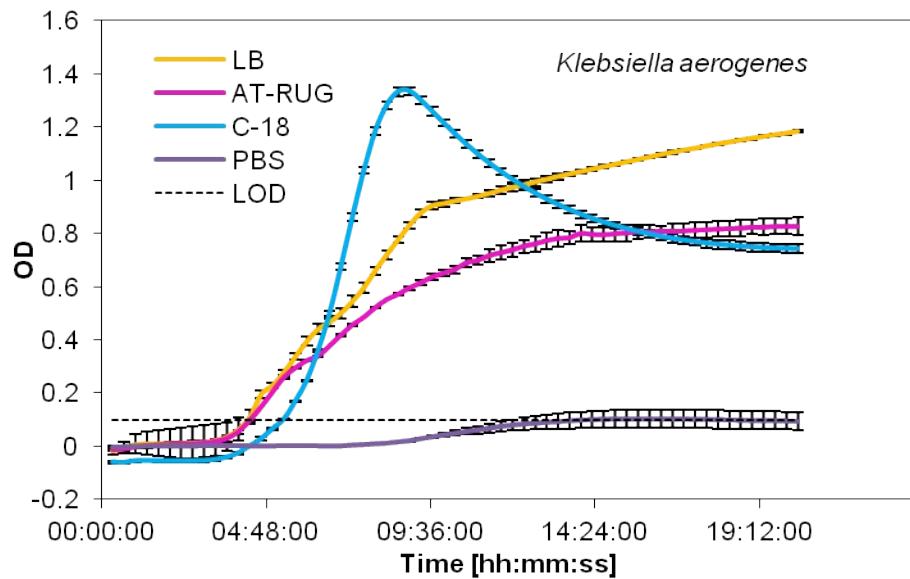


**Fig. S6** Growth curve of *Klebsiella aerogenes* in different media measured at 365 nm.

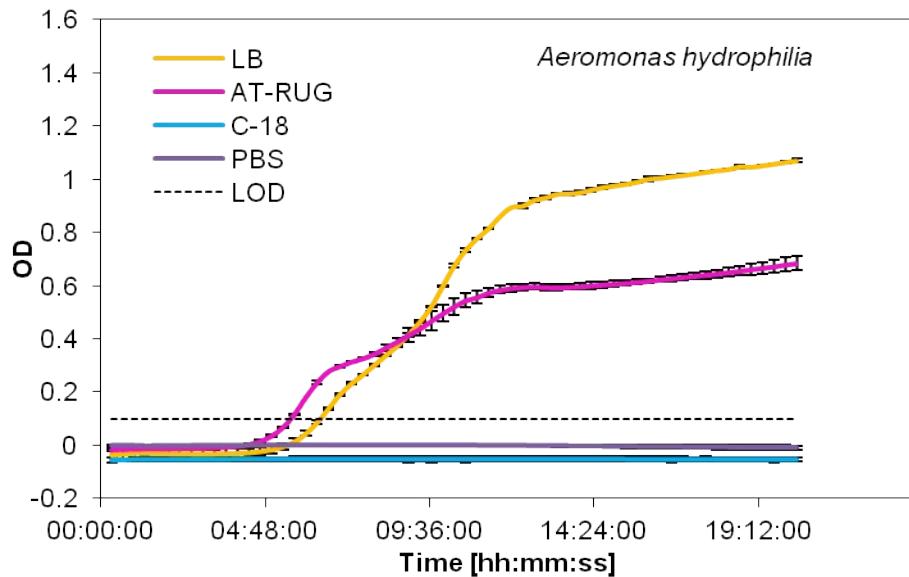

**Fig. S7** Growth curve of *Aeromonas hydrophilia* in different media measured at 365 nm.

### Temperate study Switzerland

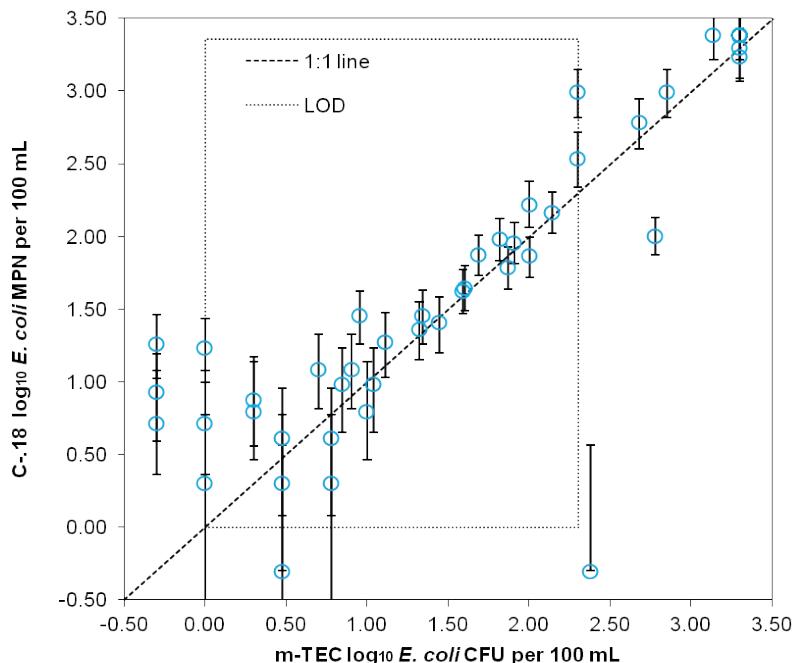

**Fig. S8** Scatter plot of C-18 *E. coli* estimates with 95 % confidence intervals versus m-TEC. Confidence intervals are only valid in the range of detection.

**Table S1** Results of paired samples t-test including t-value, p-value, 95 % confidence interval (CI) and mean difference ( $\mu_d$ ) of AT-RUG and m-TEC *E. coli* estimates.

	m-TEC			
	t	p-value	$\mu_d$	95 % CI
<b>Two-tailed <math>H_1</math></b> $\mu_d \neq 0$	1.013	0.315	0.066	[-0.064, 0.196]
<b>Upper-tailed <math>H_1</math></b> $\mu_d > 0$	1.013	0.158	0.066	[-0.043, Inf]
<b>Lower-tailed <math>H_1</math></b> $\mu_d < 0$	1.013	0.842	0.066	[-Inf, 0.175]

**Table S2** Results of paired samples t-test including t-value, p-value, 95 % confidence interval (CI) and mean difference ( $\mu_d$ ) of AT-RUG and C-18 *E. coli* estimates.

C-18		t	p-value	$\mu_d$	95 % CI
<b>Two-tailed <math>H_1</math></b> $\mu_d \neq 0$	-1.122	0.267	-0.033		[-0.092, 0.026]
<b>Upper-tailed <math>H_1</math></b> $\mu_d > 0$	-1.122	0.867	-0.033		[-0.082, Inf]
<b>Lower-tailed <math>H_1</math></b> $\mu_d < 0$	-1.122	0.133	-0.033		[-Inf, 0.016]

**Table S3** Comparison of categorical concentrations of *E. coli* from C-18 using Quanti-Tray®/2000 system and m-TEC using membrane filtration. Percentages refer to the total sampling number.

C-18 (MPN/100 mL)	m-TEC (CFU/100 mL)					Total
	<1	1 - 10	11 - 100	>100		
<1	<b>0 % (0)</b>	1.45 % (1)	0 % (0)	1.45 % (1)		2.9 % (2)
1 - 10	2.9 % (2)	<b>14.49 % (10)</b>	1.45 % (1)	0 % (0)		18.84 % (14)
11 - 100	1.45 % (1)	5.8 % (4)	<b>14.49 % (10)</b>	1.45 % (1)		23.19 % (14)
>100	0 % (0)	0 % (0)	0 % (0)	<b>55.07 % (38)</b>		55.07 % (39)
Total	4.35 % (3)	21.74 % (15)	15.94 % (11)	57.97 % (40)		100 % (69)

**Table S4** Comparison of AT-RUG and m-TEC results based on sample positivity for *E. coli*


AT-RUG (MPN/100 mL)	m-TEC (CFU/100 mL)		
	Negative	Positive	Total
Negative	0 % (0)	100 % (2)	100 % (2)
Positive	4.5 % (3)	95.5 % (64)	100 % (67)
Total	4.3 % (3)	95.7 % (66)	100 % (69)

**Table S5** Comparison of AT-RUG and C-18 results based on sample positivity for *E. coli*


AT-RUG (MPN/100 mL)	C-18 (MPN/100 mL)		
	Negative	Positive	Total
Negative	50 % (1)	50 % (1)	100 % (2)
Positive	1.5 % (1)	98.5 % (66)	100 % (67)
Total	2.9 % (2)	97.1 % (67)	100 % (69)

**Table S6** Comparison of C-18 and m-TEC results based on sample positivity for *E. coli*


C-18 (MPN/100 mL)	m-TEC (CFU/100 mL)		
	Negative	Positive	Total
Negative	0 % (0)	100 % (2)	100 % (2)
Positive	4.5 % (3)	95.5 % (64)	100 % (67)
Total	4.3 % (3)	95.7 % (66)	100 % (69)

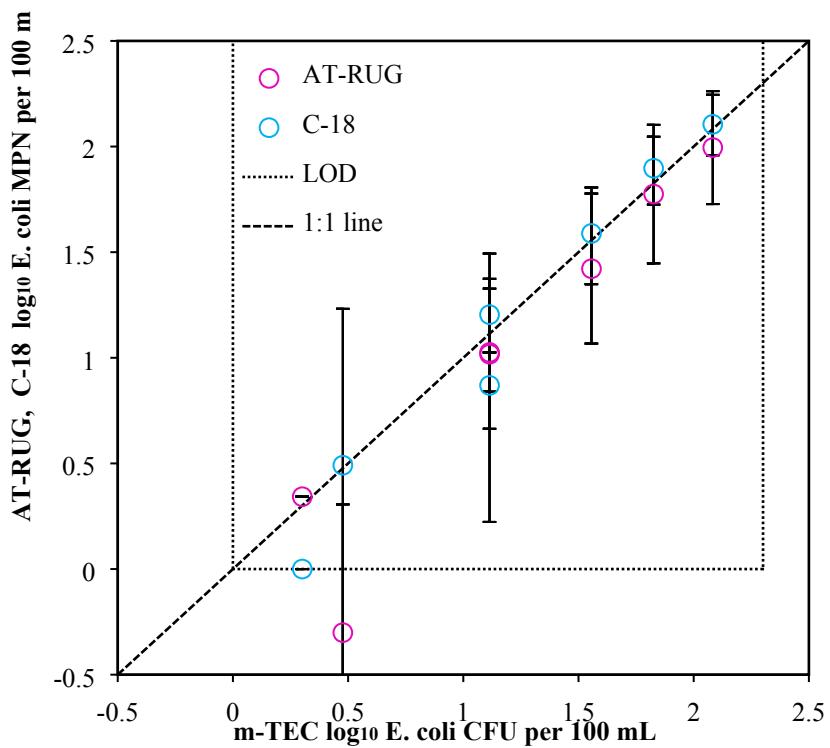

**Fig. S9** Laboratory comparison of AT-RUG and C-18  $E. coli$  estimates with 95 % confidence intervals versus m-TEC. Confidence intervals are only valid in the range of detection.

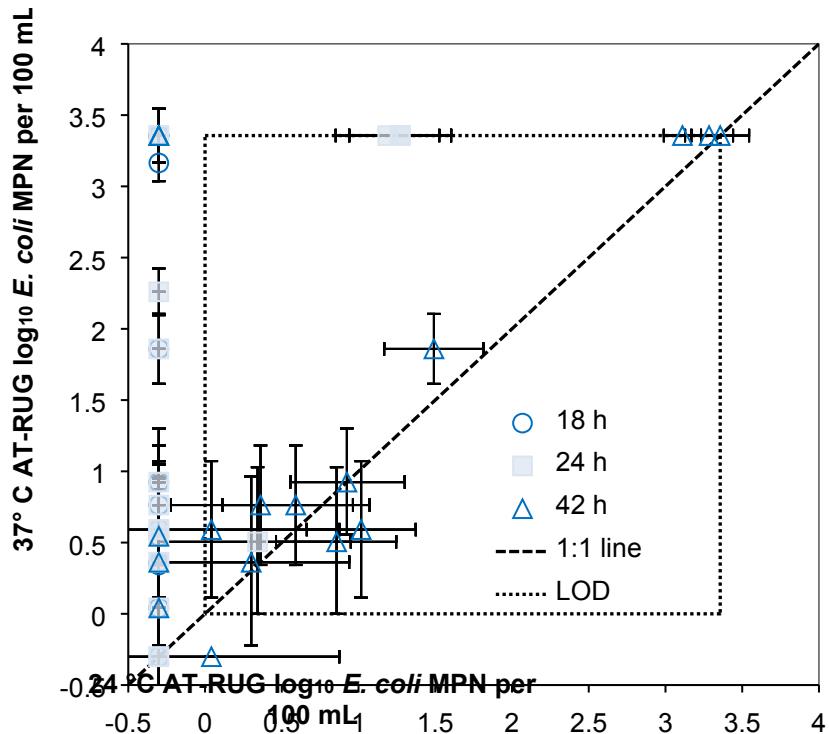

**Fig. S10** Scatter plot of AT-RUG  $E. coli$  estimates at  $24^\circ\text{C}$  with 95 % confidence intervals versus AT-RUG at  $37^\circ\text{C}$ . Confidence intervals are only valid in the range of detection.

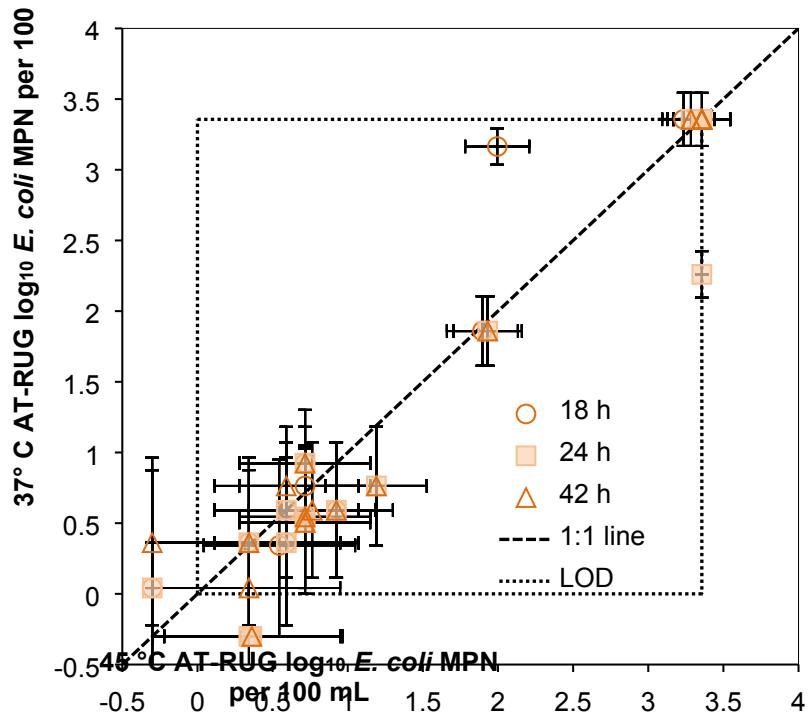

**Fig. S11:** Scatter plot of AT-RUG *E. coli* estimates at 45 °C with 95 % confidence intervals versus AT-RUG at 37 °C. Confidence intervals are only valid in the range of detection.

## Tropical study Uganda

**Table S7** Results of paired samples t-test including t-value, p-value, 95 % confidence interval (CI) and mean difference ( $\mu_d$ ) of AT-RUG and m-ColiBlue24® *E. coli* estimates

	m-ColiBlue24®			
	t	p-value	$\mu_d$	95 % CI
<b>Two-tailed <math>H_1</math></b> $\mu_d \neq 0$	2.451	0.016	0.116	[0.022, 0.210]
<b>Upper-tailed <math>H_1</math></b> $\mu_d > 0$	2.451	0.008	0.116	[-0.037, Inf]
<b>Lower-tailed <math>H_1</math></b> $\mu_d < 0$	2.451	0.992	0.116	[-Inf, 0.195]

**Table S8** Comparison of AT-RUG and m-ColiBlue24® results based on sample positivity for *E. coli*

AT-RUG (MPN/100 mL)	m-ColiBlue24® (CFU/100 mL)		
	Negative	Positive	Total
Negative	77.8 % (14)	22.2 % (4)	100 % (18)
Positive	4.5 % (3)	95.5 % (64)	100 % (67)
Total	20.0 % (17)	95.5 % (68)	100 % (85)