

Supplementary Informations

Fig.1 The calibration curve for the linear relationship between the standard concentration of fluoride ion and the electrode potential:

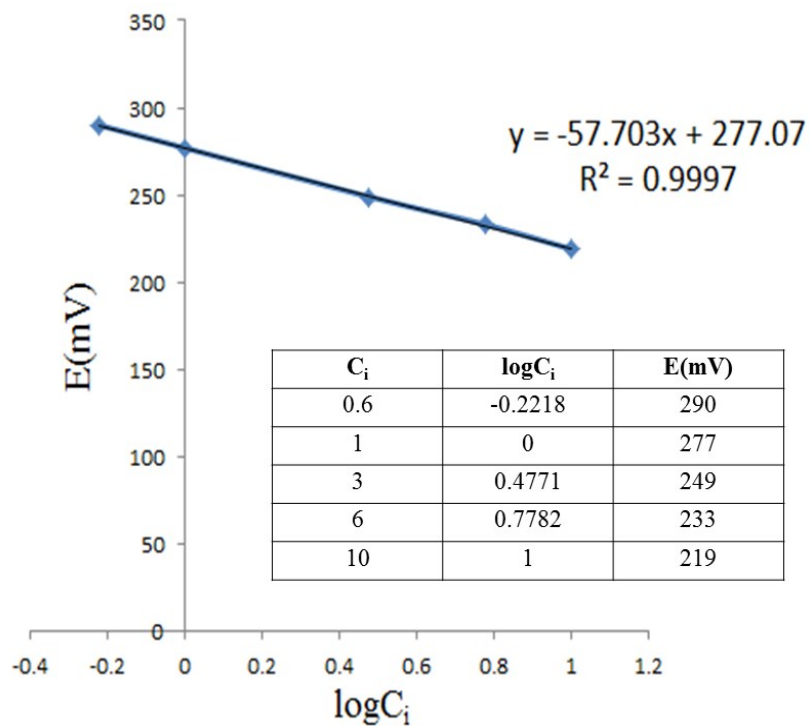


Fig.2 Zeta potential of the Zr-GP gel at different pH values

