

A new approach towards simultaneous extraction of individual analytes based on the simultaneous application of multiple magnetic sorbents

Mohammad Reza Fattahi Bafghi, Shayessteh Dadfarnia*, Ali Mohammad Haji Shabani, Elahe Kazemi, Mahnaz Nozohour Yazdi

Department of Chemistry, Faculty of Science, Yazd University, Safaieh, 89195-741, Yazd, Iran

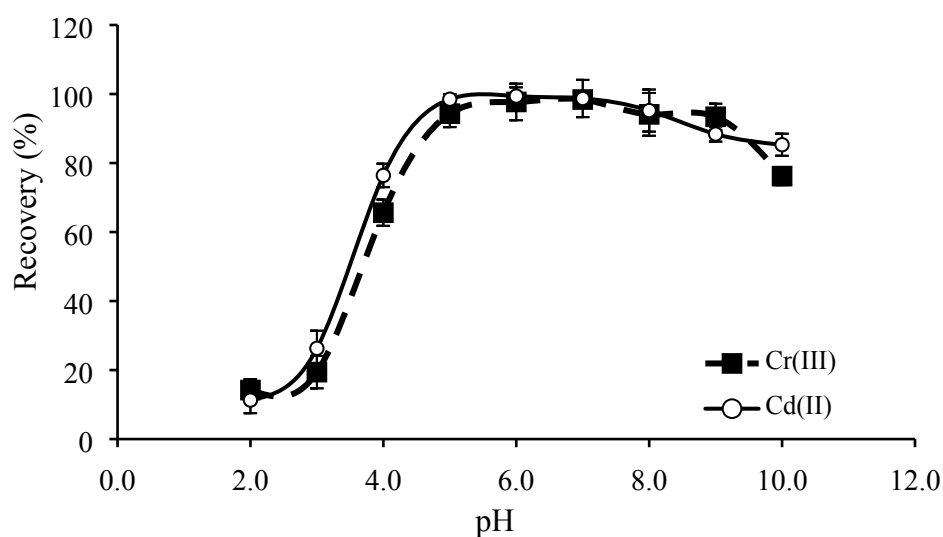


Fig. S1: Effect of sample pH on the extraction. Conditions: sample volume, 40 mL; amount of sorbent, 40 mg; sample flow rate, 2 mL min⁻¹; eluent concentration, 3.0 mol L⁻¹; eluent volume, 500 µL.

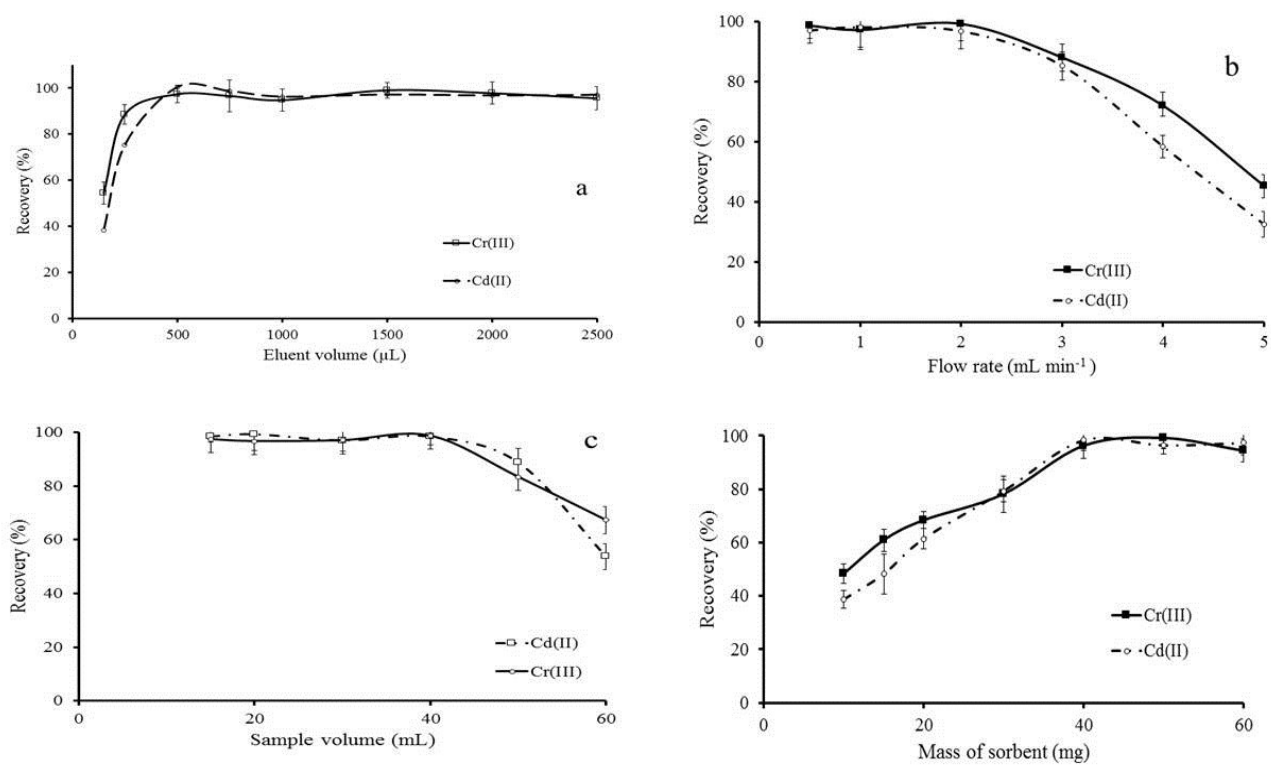


Fig. S2: Effect of eluent volume (a); sample flow rate (b), sample volume (c); and mass of sorbent (d): Conditions: pH, 6; eluent concentration, 3.0 mol L^{-1} .

