


Electronic Supplementary Information_1

Emission spectra of a dedicated custom-made high-power COB LED light source determined by a spectroradiometer GL Spectis 5.0 Touch.

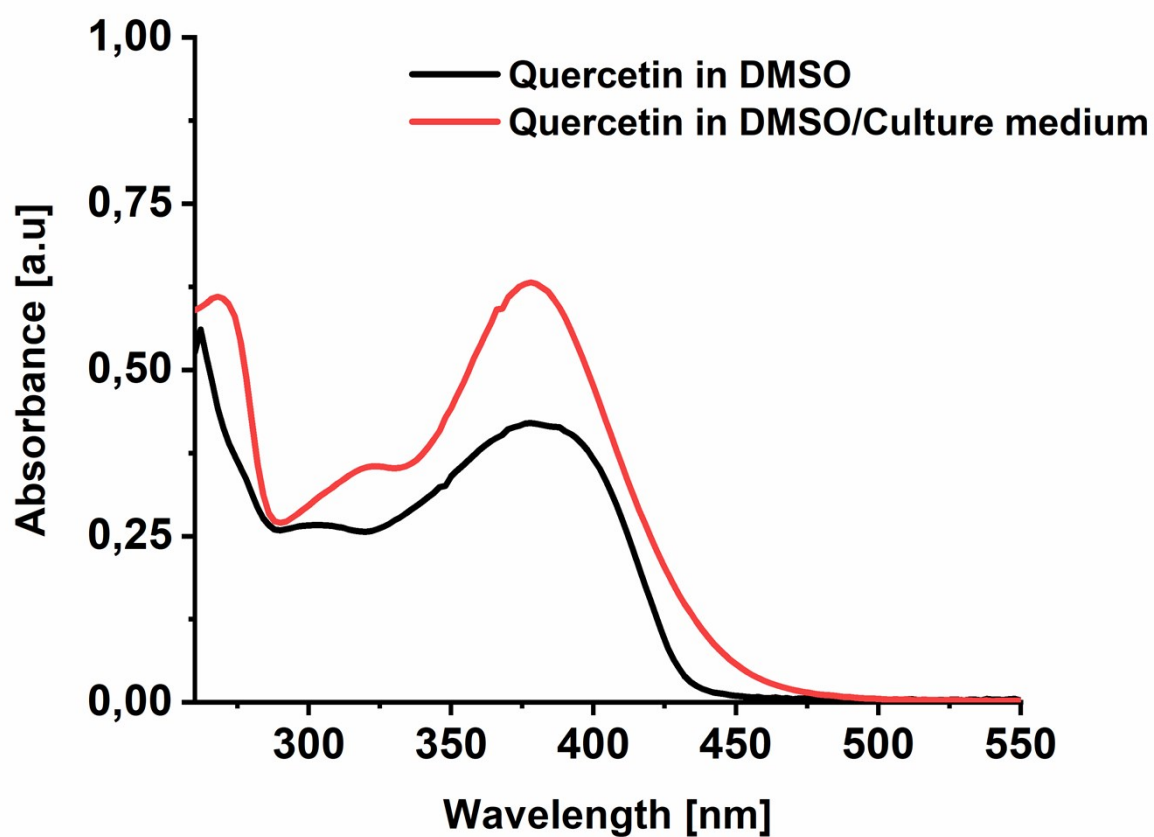

Electronic Supplementarny Information_2

Spectroscopic analyzes of quercetin solutions prepared in DMSO and in DMSO diluted in cell culture medium.