

Design of An electrochemical platform for Determination of Diclofenac Sodium utilizing a Graphenized Pencil Graphite Electrode Modified with Cu-Al Layered Double Hydroxide/ Chicken Feet Yellow Membrane

Younes Bahadori*, Habib Razmi*

Department of Chemistry, Faculty of Basic Sciences, Azarbaijan Shahid Madani University, P.O.

Box 53714-161, Tabriz, Iran

Table of Contents

Fig. S1. Optimization of parameters influencing the preparation of Cu-Al LDH/CFYM/GPGE based on DCF oxidation response ($[DCF] = 47.6 \mu\text{M}$: (A) influence of concentration of CFYM, and (B) influence of concentration of Cu-Al LDH dispersion.

Fig. S2. DPV current response of (A) reconstruction, (B) repeatability, and (C) storage stability on the Cu-Al LDH/CFYM/GPGE sensor in PBS solution ($\text{pH} = 7.0$) containing $47.6 \mu\text{M}$ DCF.

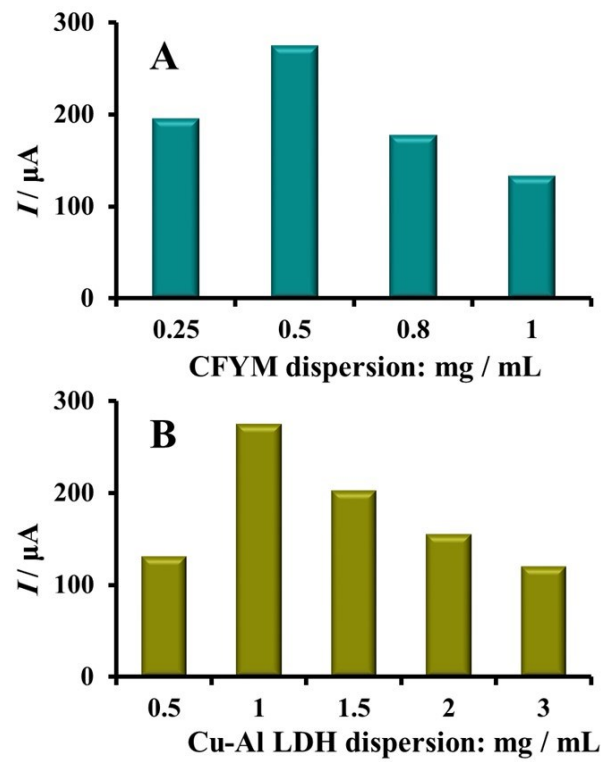


Fig. S1. Optimization of parameters influencing the preparation of Cu-Al LDH/CFYM/GPGE based on DCF oxidation response ($[\text{DCF}] = 47.6 \mu\text{M}$): (A) influence of concentration of CFYM, and (B) influence of concentration of Cu-Al LDH dispersion.

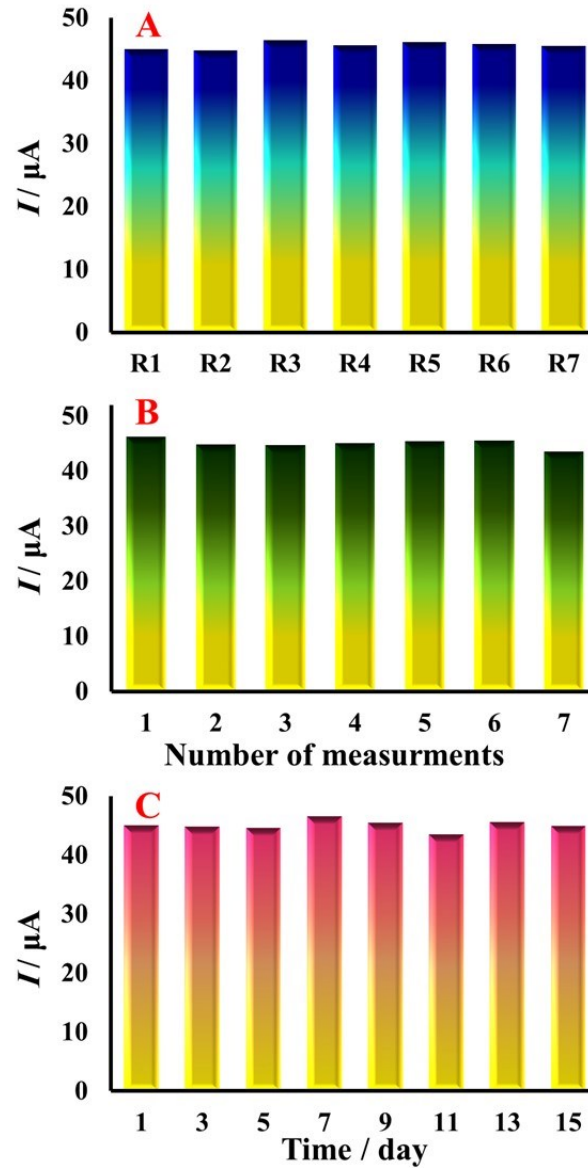


Fig. S2. DPV current response of (A) reconstruction, (B) repeatability, and (C) storage stability on the Cu-Al LDH/CFYM/GPGE sensor in PBS solution (pH = 7.0) containing 47.6 μM DCF.