



A)

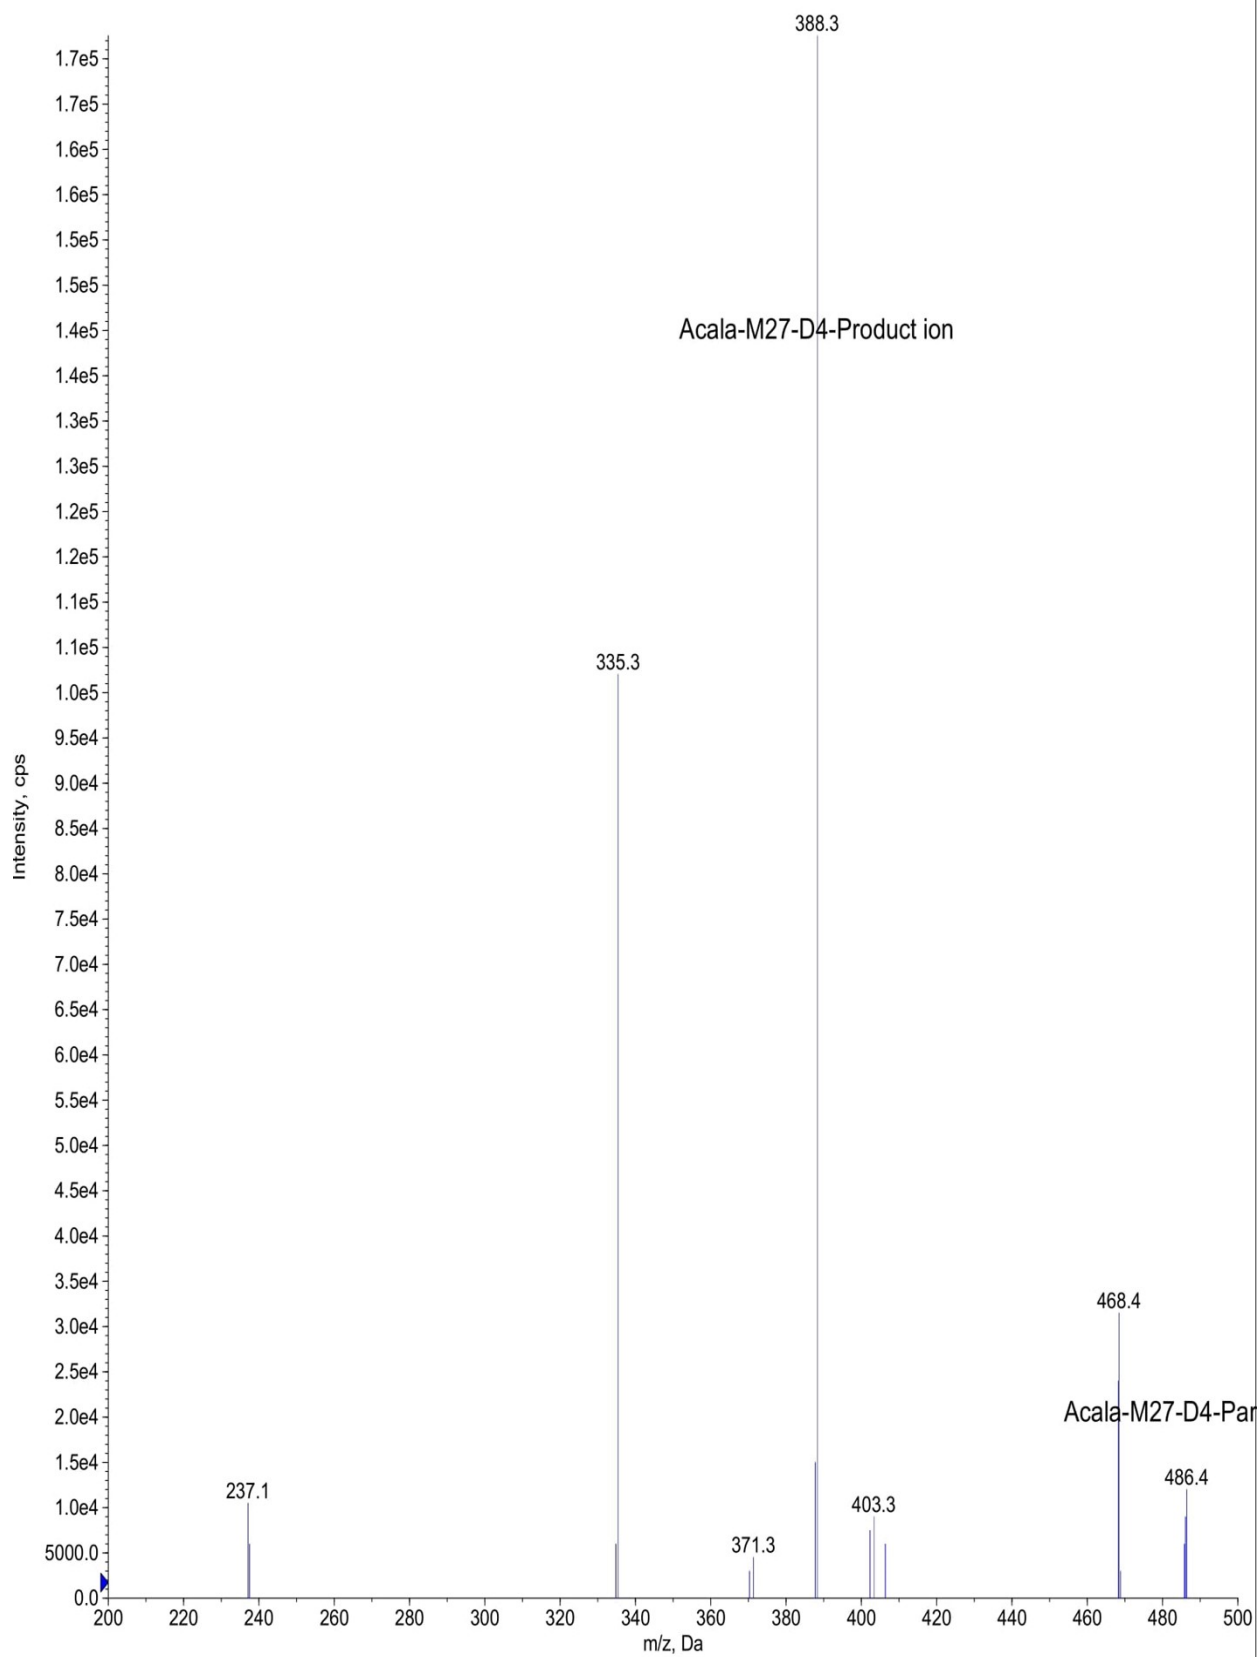

B)

+MS2 (482.30): 0.000 min from Sample 1 (TuneSampleID) of MT20210624171339.wiff (Turbo Spray), ...


Max. 1.4e5 cps

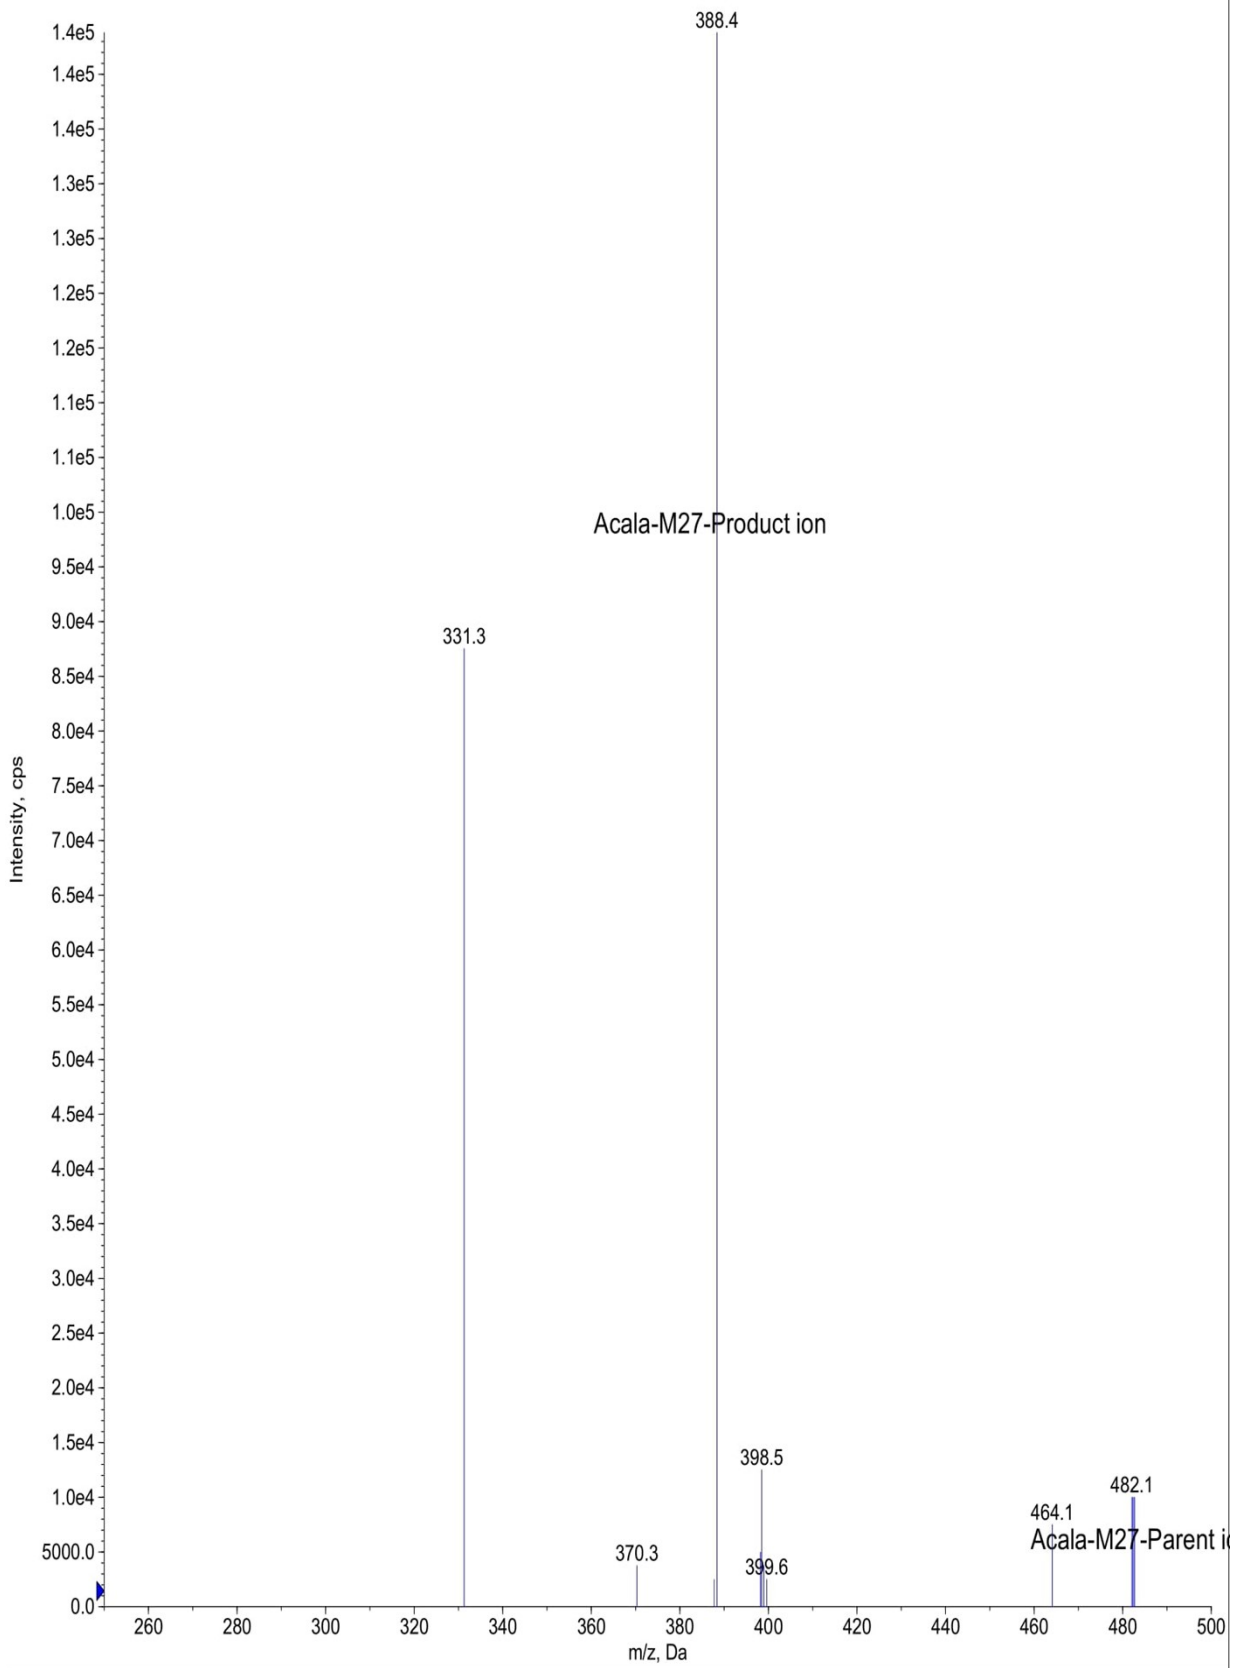

C)

■ +MS2 (466.20): 0.000 min from Sample 1 (TuneSampleID) of MT20210624144931.wiff (Turbo Spray), ...

Max. 1.4e5 cps.

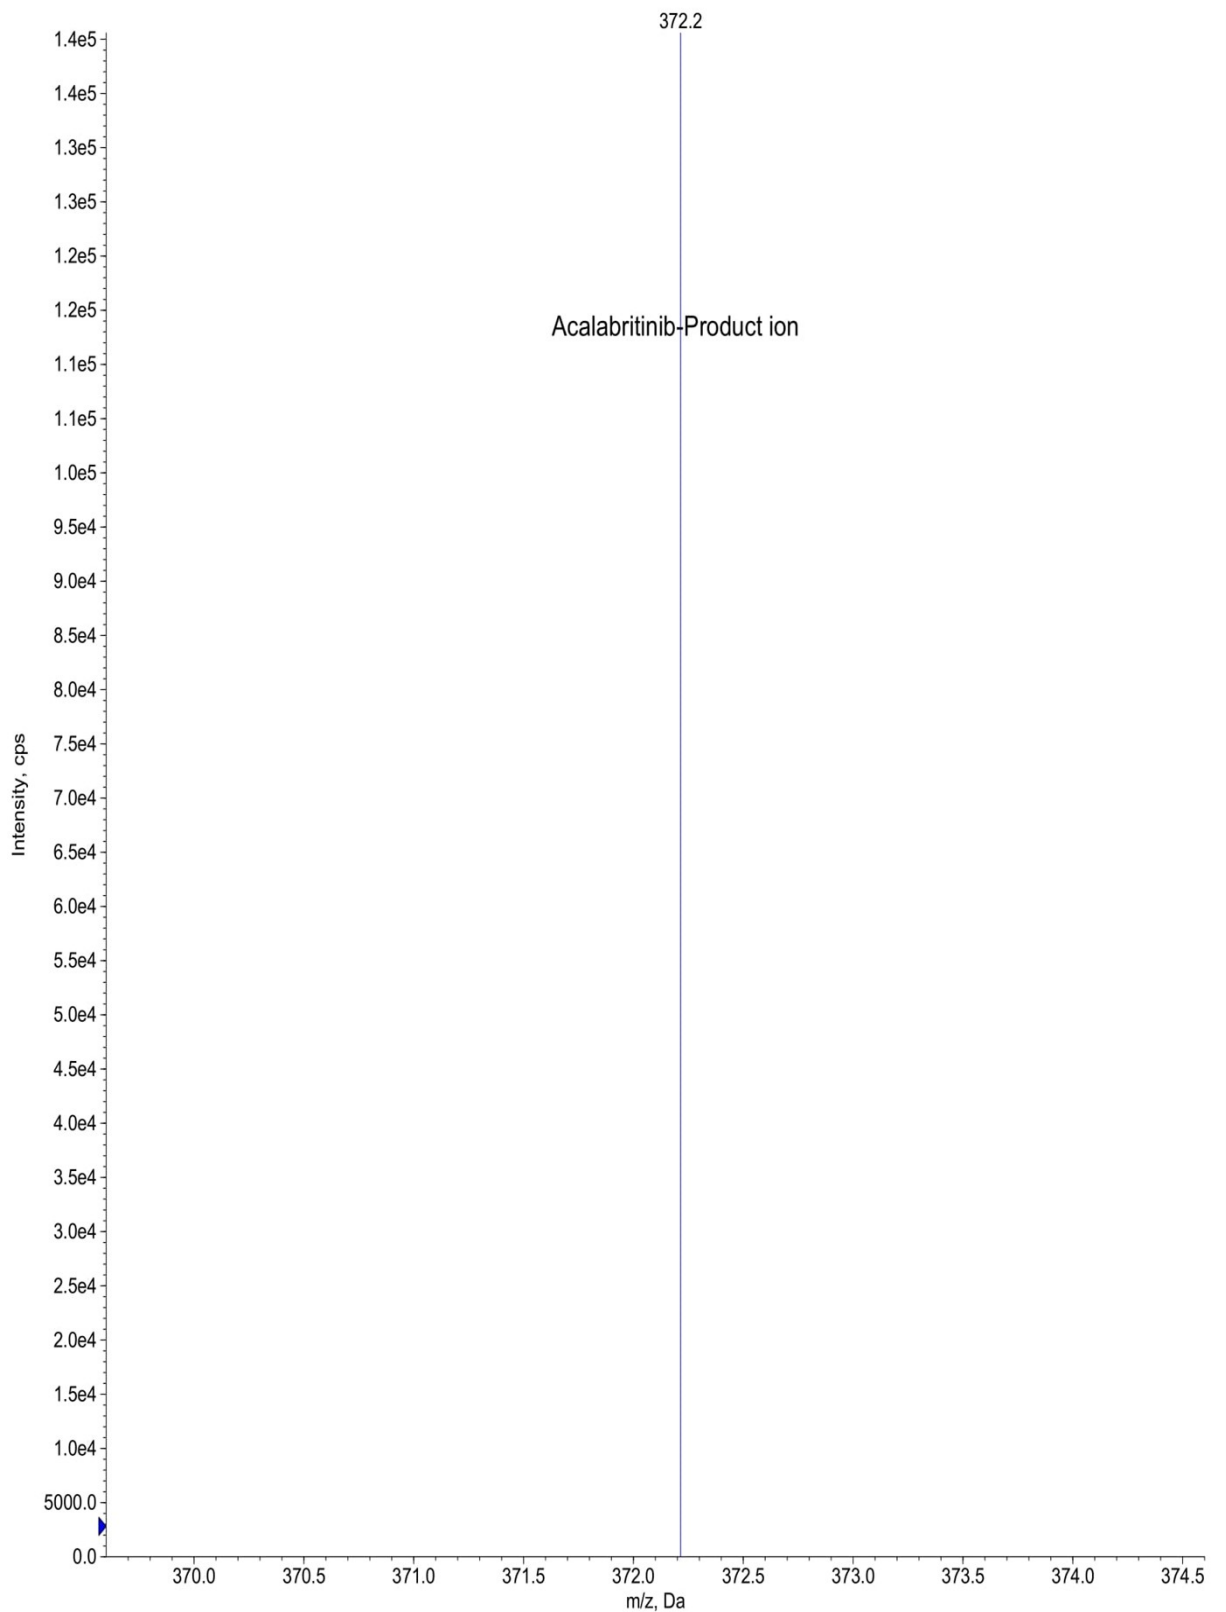

D)

Product ion mass spectrum for A) Acalabrutinib-D4, B) Acalabrutinib-M27-D4, C) Acalabrutinib-M27 and D) Acalabrutinib.