



Appendix A. Supplementary material


TEHTM metabolites

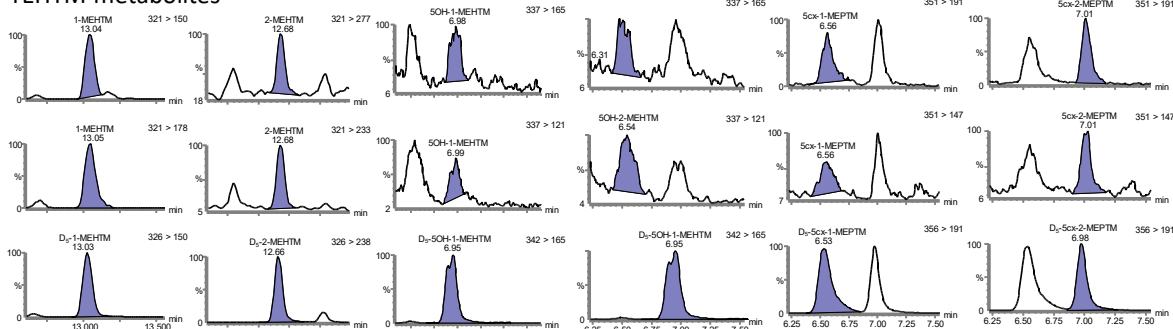


DEHP metabolites

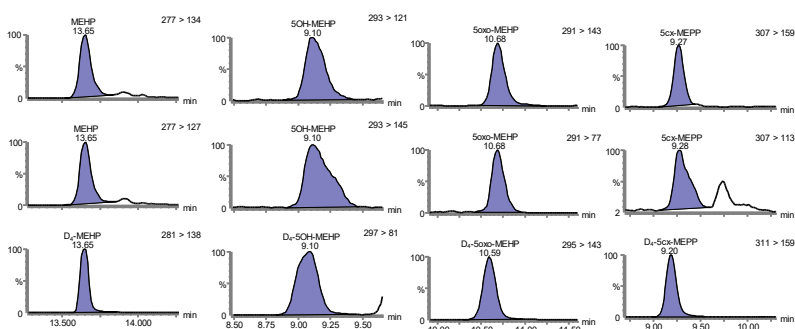

DEHTP metabolites

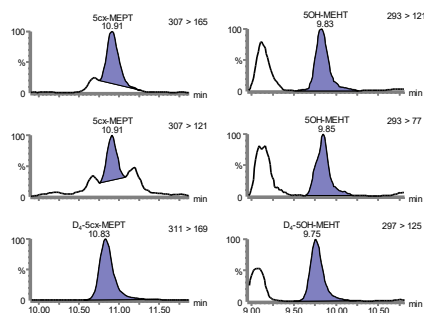

DINCH metabolites

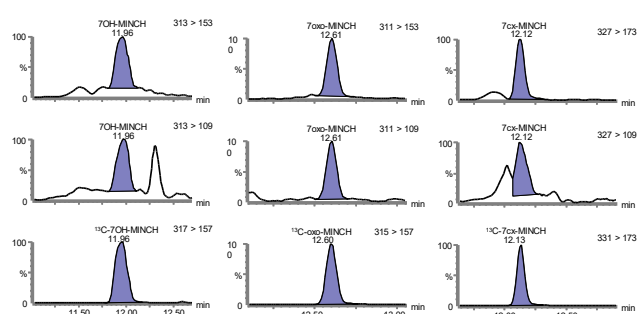

Supplemental Figure 1: Chromatograms of a spiked urine sample (lowest calibration standard) with the following spiked analyte levels: 0.1 µg/L each for all TEHTM metabolites, 0.2 µg/L each for all other analytes.