



Supplemental Figures

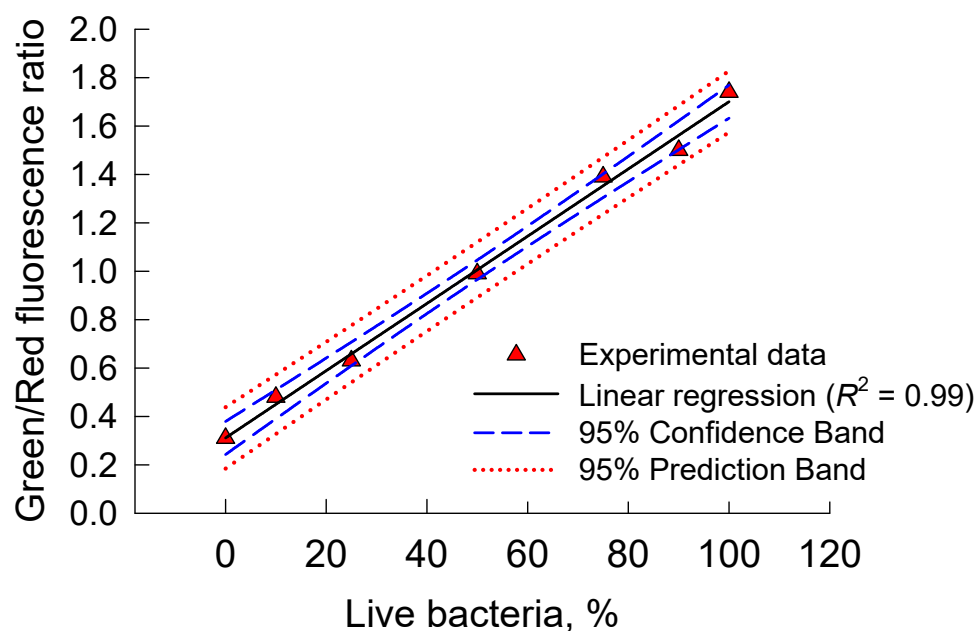

Suppl. Figure 1. Standard curve for various proportions of live/dead cells for fluorescence microplate readers.

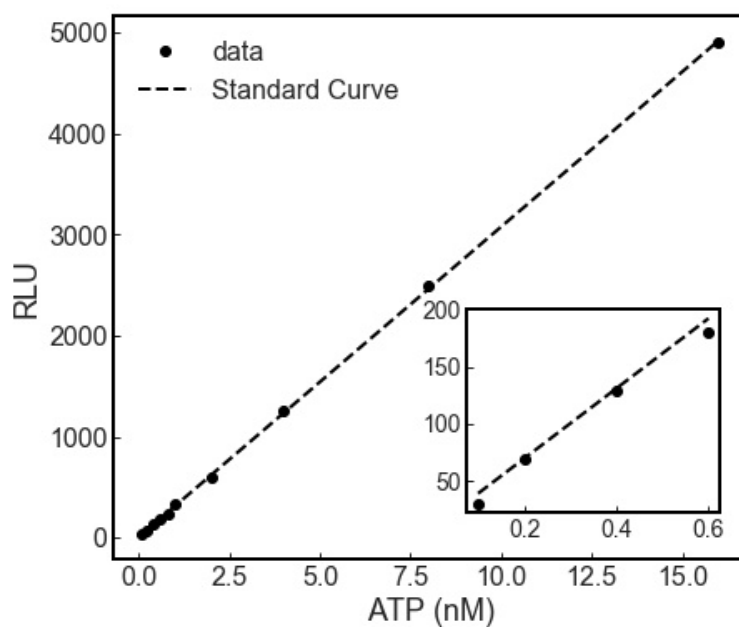

Suppl. Figure 2. Standard curve for detection of ATP using the ATP Determination Kit.