

Electrochemical sensor for the determination of environmentally hazardous fungicide pyrimethanil in water and fruit samples

Chou-Yi Hsu ^{a,*}, Tariq J. Al-Musawi ^b, Rahim Lataef ^c, Holya A. Lafta ^d, Dalal Abdullah Fatthi^e, Ahmed S. Abed ^f, Salema K. Hadrawi ^{g,*}, Maysm Barzan Talb ^h, Irfan Ahmad ⁱ, Safia Obaidur Rab ⁱ, Mohammad Y. Alshahrani ⁱ

^a *Department of Pharmacy, Chia Nan University of Pharmacy and Science, Tainan City 71710, Taiwan.*

^b *Building and Construction Techniques Engineering Department, Al-Mustaqbal University College, 51001 Hillah, Babylon, Iraq.*

^c *College of Medical Technology/ Al-Farahidi University/ Iraq*

^d *Al-Nisour University College/Baghdad/Iraq*

^e *Department of Medical Laboratory Technics, AlNoor University College, Bartella, Iraq*

^f *Hilla University college, Babylon, Iraq/ Department of Prosthetic Dental Technology/Iraq*

^g *Refrigeration and Air-conditioning Technical Engineering Department, College of Technical Engineering, The Islamic University, Najaf, Iraq*

^h *Mazaya University College/ Iraq*

ⁱ *Department of Clinical Laboratory Sciences, College of Applied Medical Sciences, King Khalid University, Abha, Saudi Arabia*

***Corresponding Authors:** Email: drchouyihsu@gmail.com, sahadrawi@gmail.com

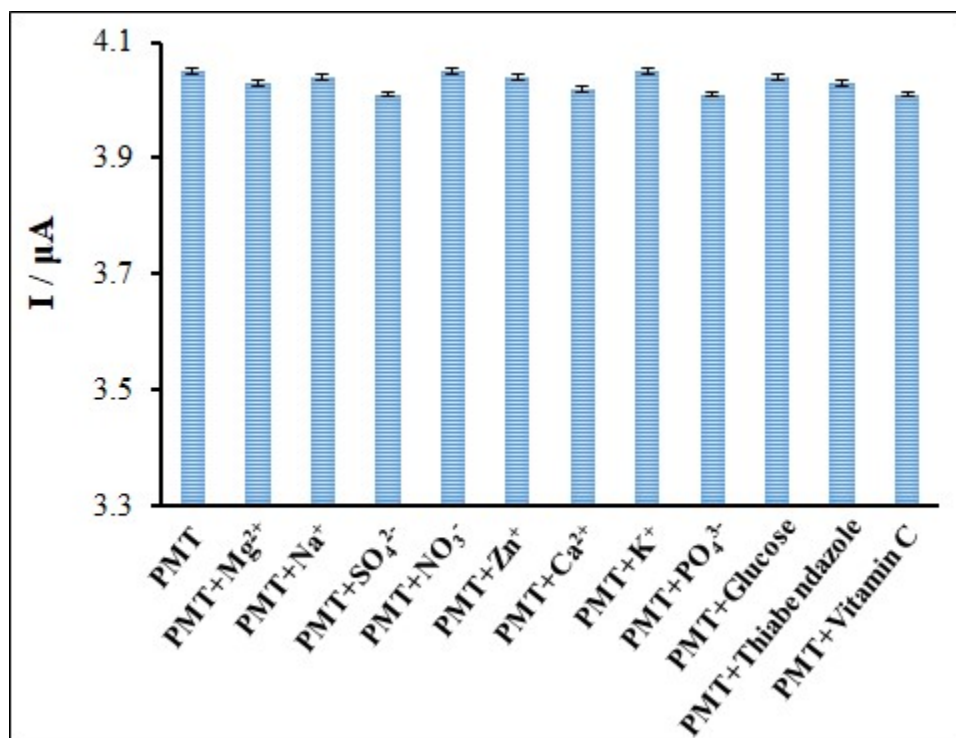


Figure S1. The oxidation current diagram of modified electrode in the presence of 50.0 μM PMT in PBS (0.1 M, pH 4) and other investigated interferences.

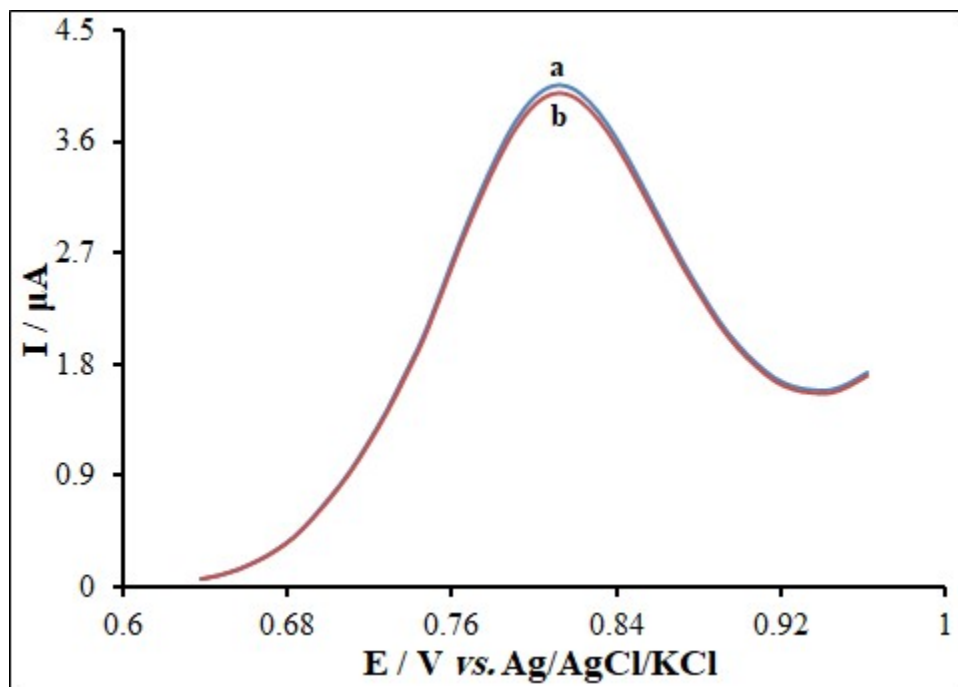


Figure S2. DPVs of modified electrode (a) (containing 20.0 μM of PMT) and (b) after four weeks.

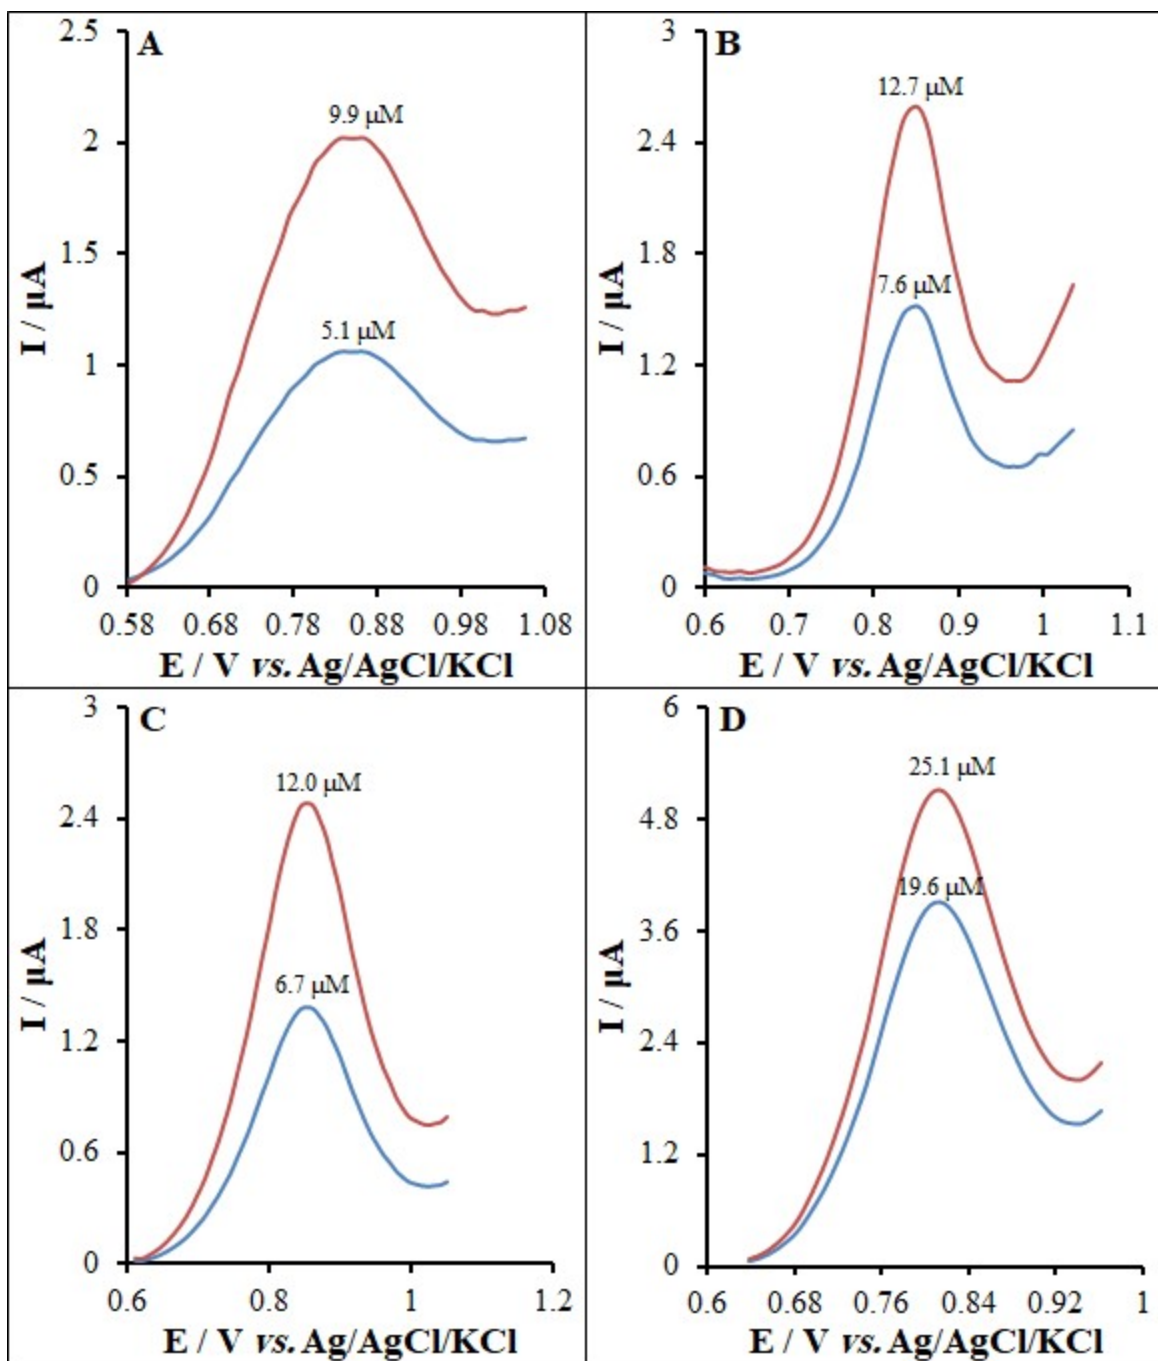


Figure S3. DPV results obtained for (A) apple, (B) orange, (C) strawberry and (D) water samples in presence of PMT at the electrode modified.