

Supplementary information

CD133-targeted multifunctional nanomicelles for dual-modality imaging and synergistic high-intensity focus ultrasound (HIFU) ablation on pancreatic cancer in nude mice

Yijing Yao[‡], Yiwen Zheng[‡], Mingtai Wu[‡], Yihui Gao, Qian Yu, Mengyao Liu, Xiaoxiao Luo, Rui Wang^{*}, Lixin Jiang^{*}

Department of Ultrasound, Renji Hospital, Shanghai Jiao Tong University School of Medicine, Shanghai 200127, China.



Fig. S1 Preparation of the window chamber

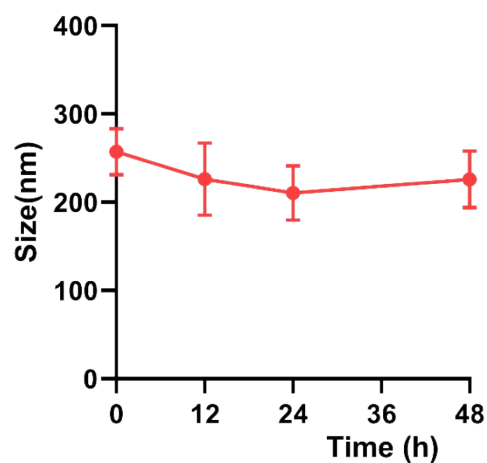


Fig. S2 Stability assessment of CD133-FITC/PFH@OSMs immersed in PBS at different time points.

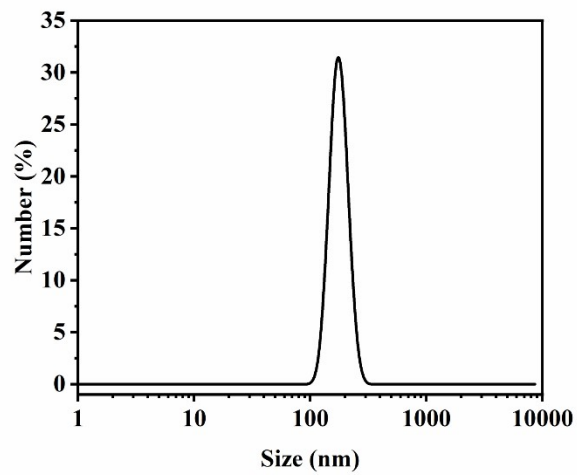


Fig. S3 Dynamic Light Scattering was used to detect the particle size distribution of CD133-FITC/PFH@OSMs.

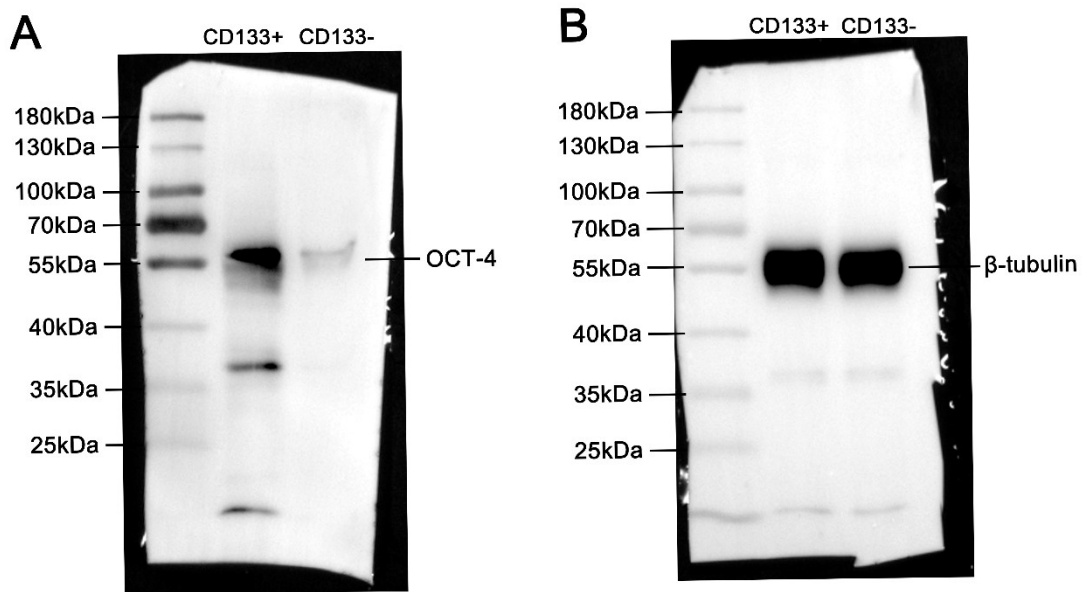


Fig. S4 The original data for the western blot results in Figure 3E.