

Figure S1

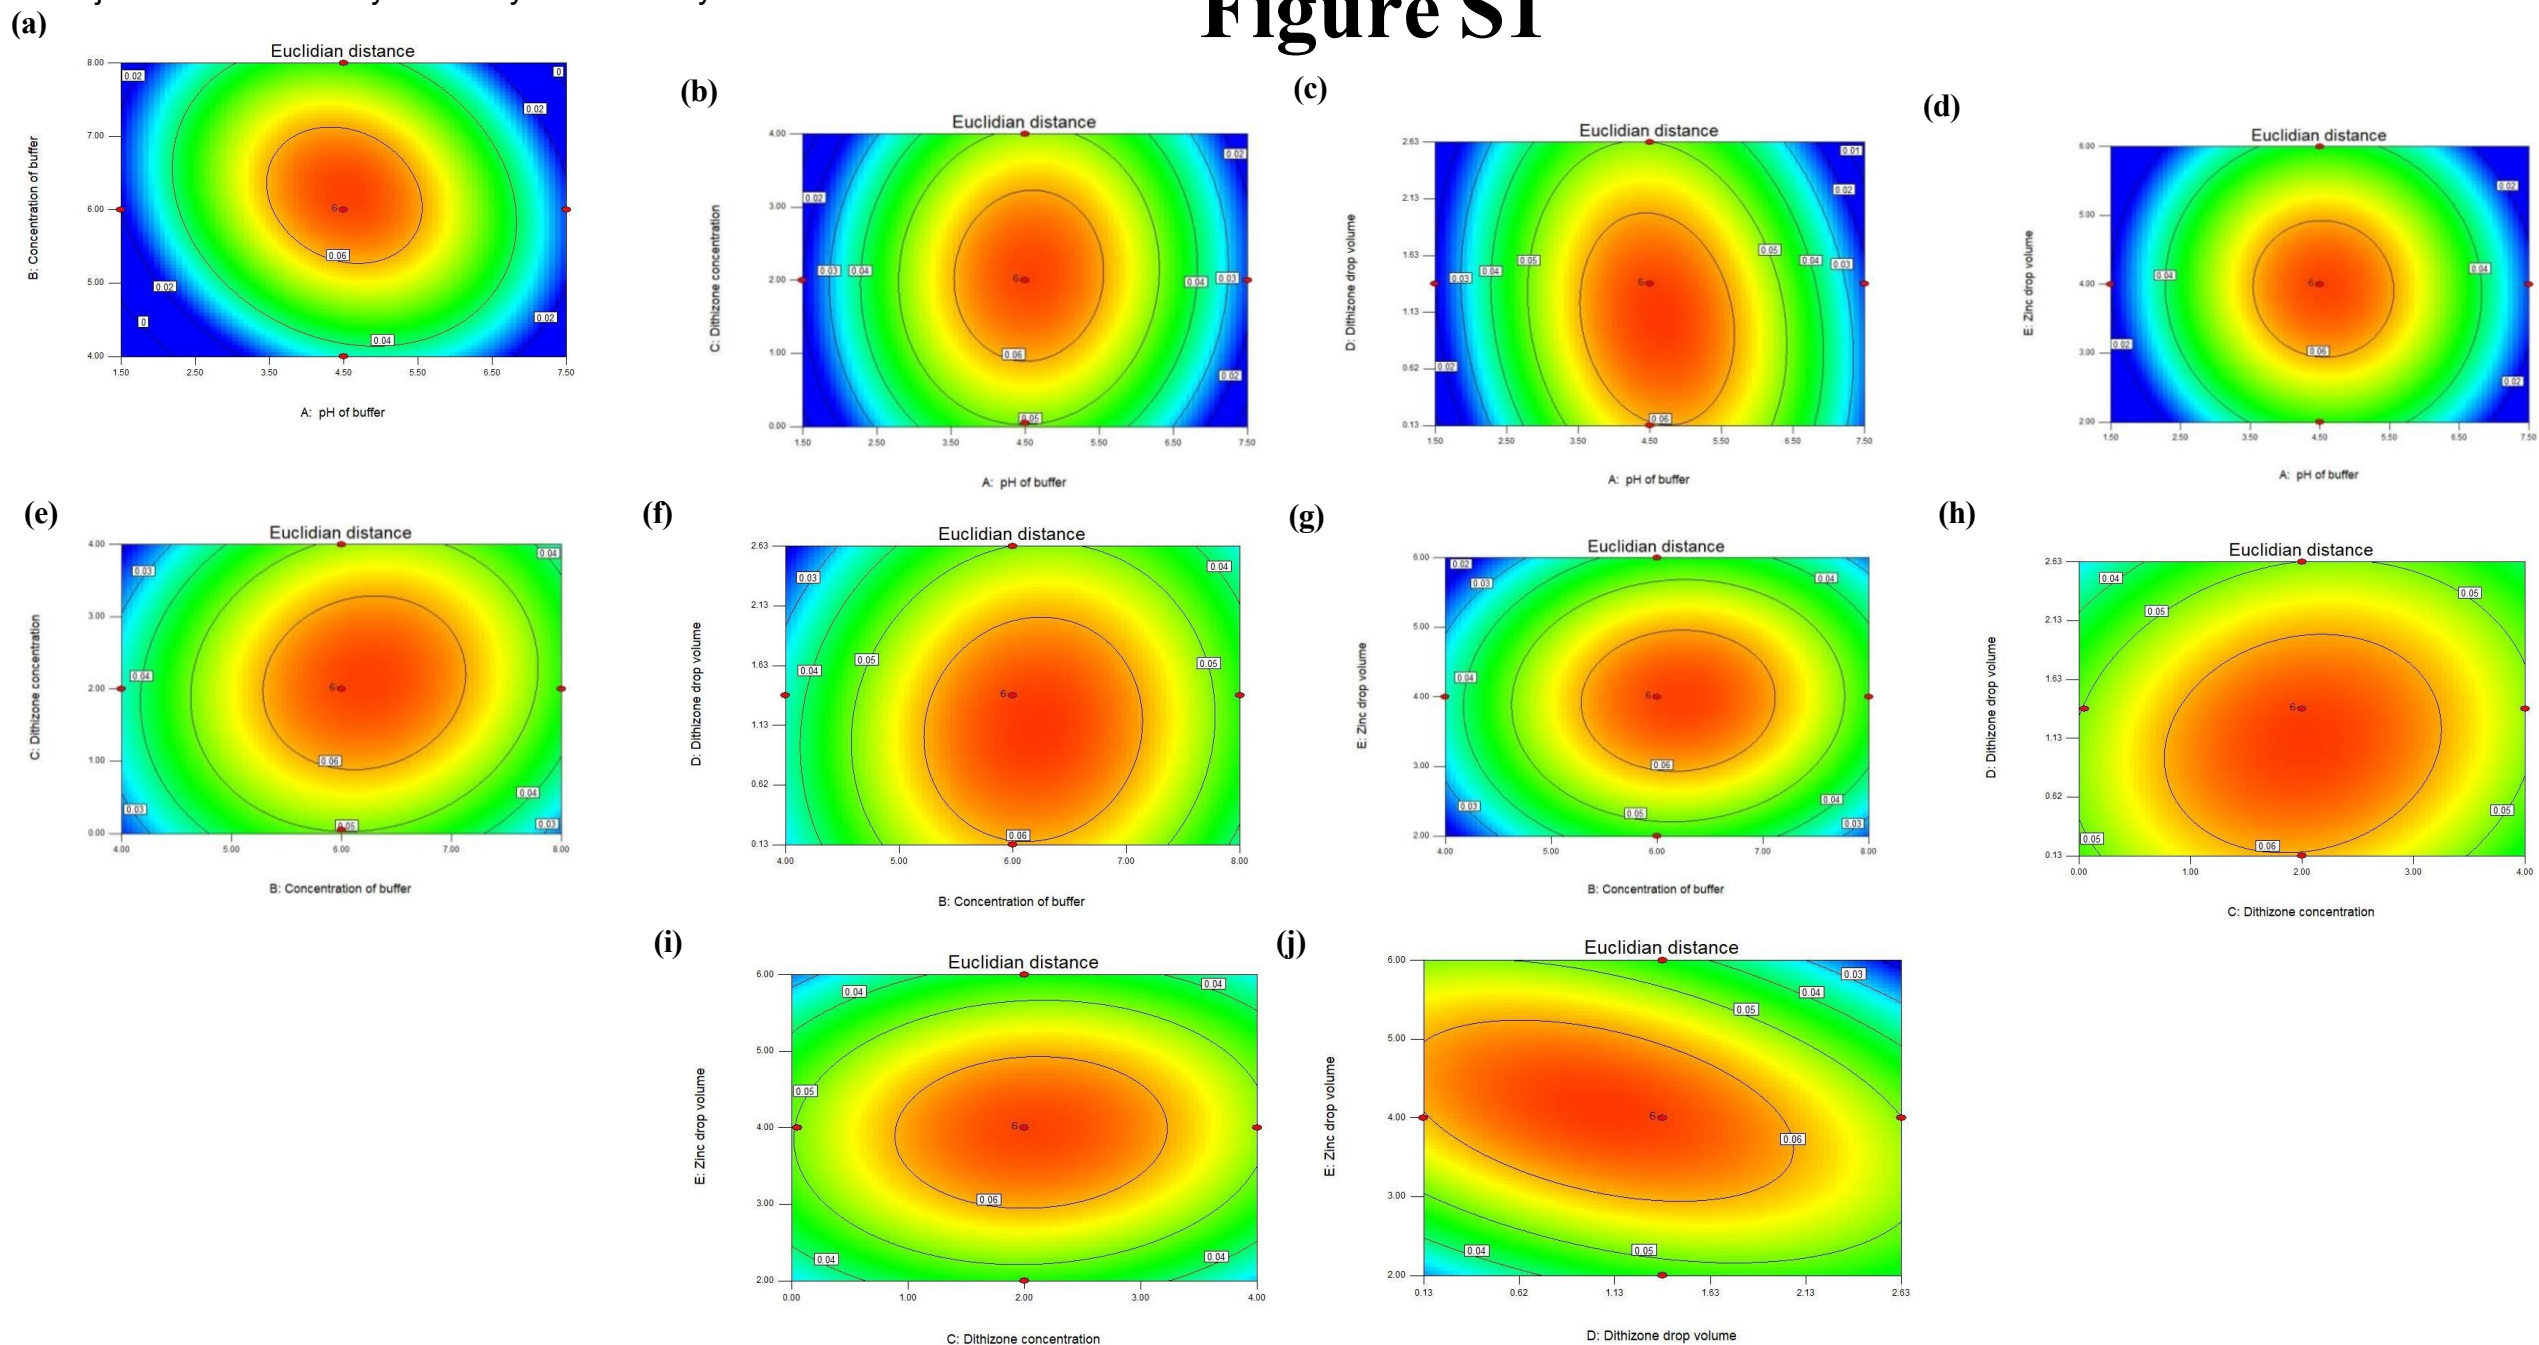


Figure S2 (a)




Figure S2 (b)


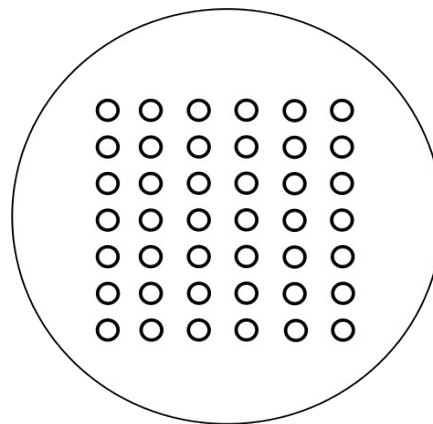


Figure S3

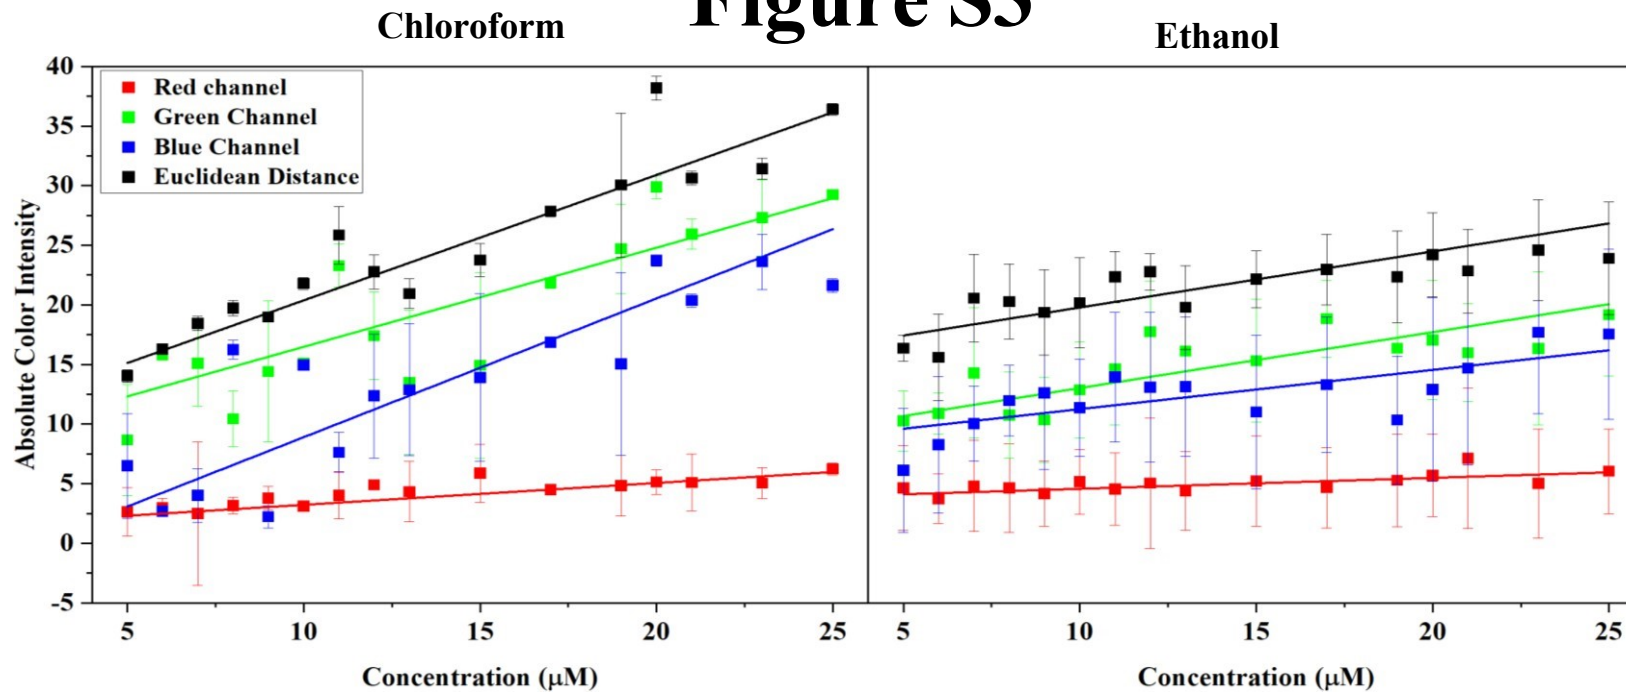

Intensity measures	Coefficient of linearity (R ²)		Mean standard deviation (mean SD)		Mean square error (MSE)		Intraclass Correlation Coefficient (ICC)		
	Solvent	Chloroform	Ethanol	Chloroform	Ethanol	Chloroform	Ethanol	Chloroform	Ethanol
Δ□		0.920	0.546	21.4	16.8	13.73	13.27	0.31	0.055
Δ□		0.922	0.735	24.9	31.7	22.36	46.76	0.29	0.03
Δ□		0.88	0.485	27.8	32.9	24.37	49.88	0.33	0.048
Δ□		0.952	0.727	16.03	41.6	9.18	73.46	0.76	0.08

Figure S4

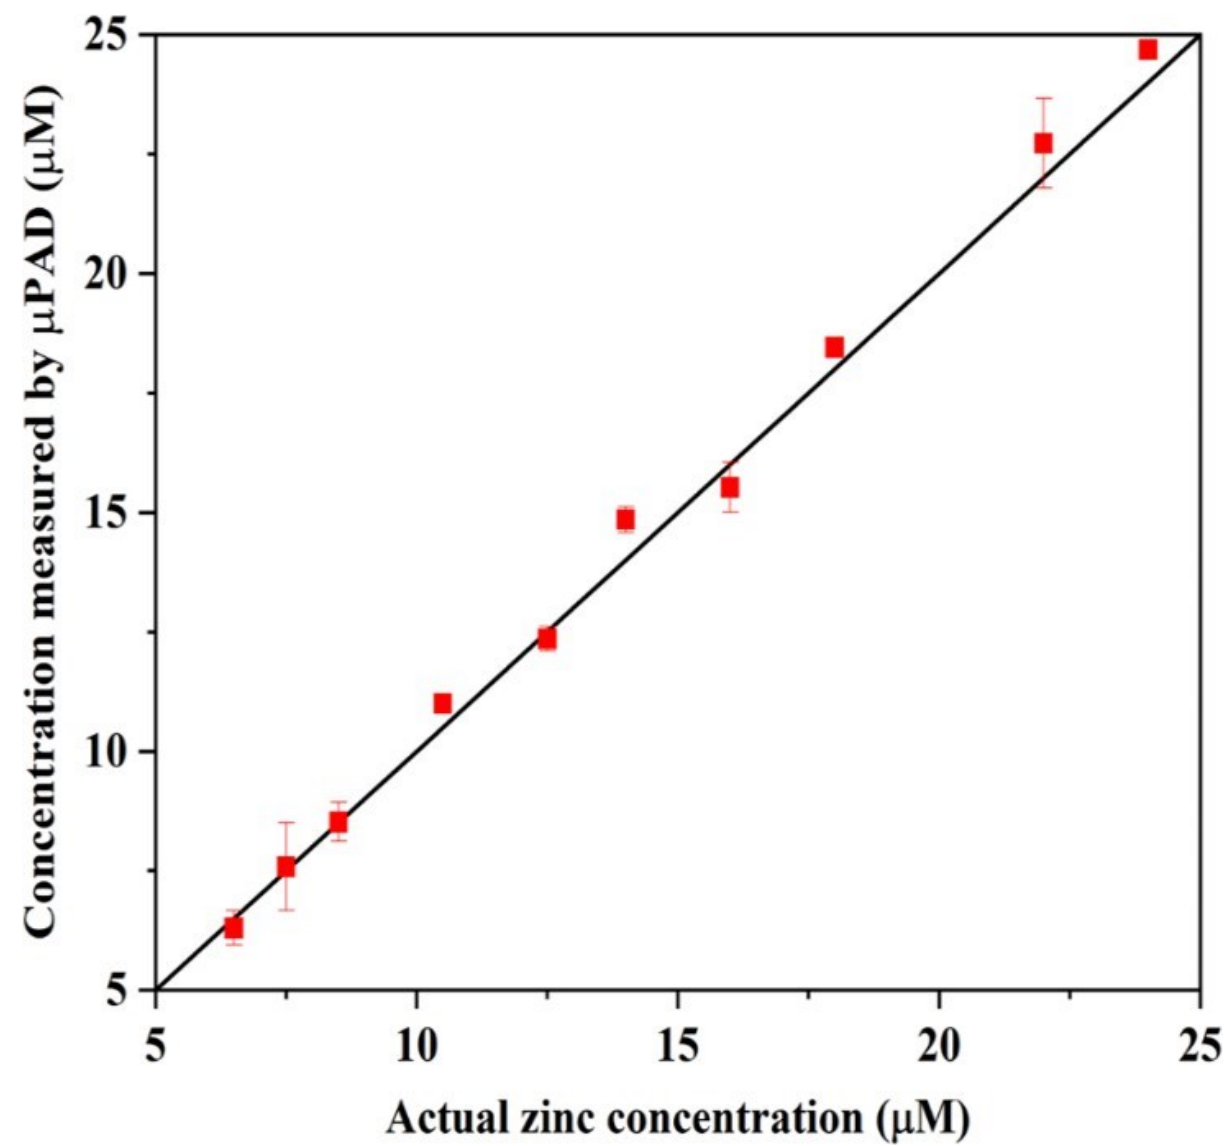


Figure S5

