

A direct solid sampling approach for fluorine determination via ETV/ICP-QQQ-MS

Vera M. Scharek¹, Heike Traub¹, Björn Meermann^{1*}

¹ Federal Institute for Materials Research and Testing (BAM), Division 1.1 – Inorganic Trace Analysis (ITALab), Richard-Willstätter-Straße 11, 12489 Berlin

*Corresponding author: PD Dr. habil. Björn Meermann, Email: bjoern.meermann@bam.de

Keywords: Fluorine, PTFE, Fractionation, Standard addition, ETV/ICP-QQQ-MS

Supporting Information:

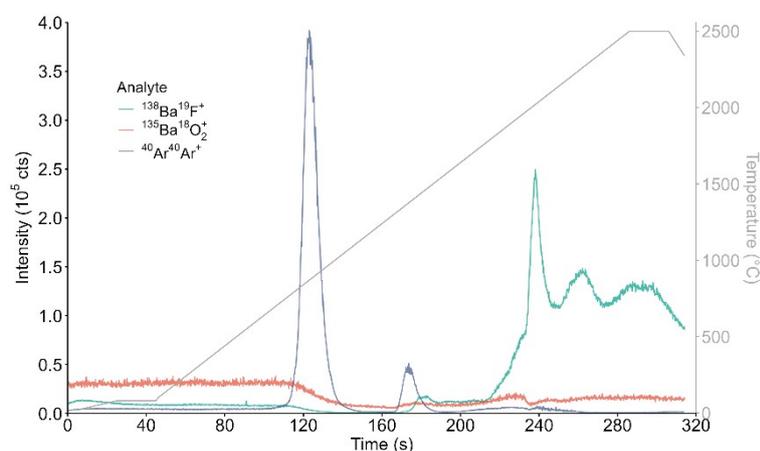


Fig. S1: ETV/ICP-QQQ-MS time scan of cyclonic dust (without standard addition) acquired in MS/MS scan mode. The CRC was pressured with an oxygen gas flow of 0.03 mL min⁻¹. The ETV temperature program is shown in grey.

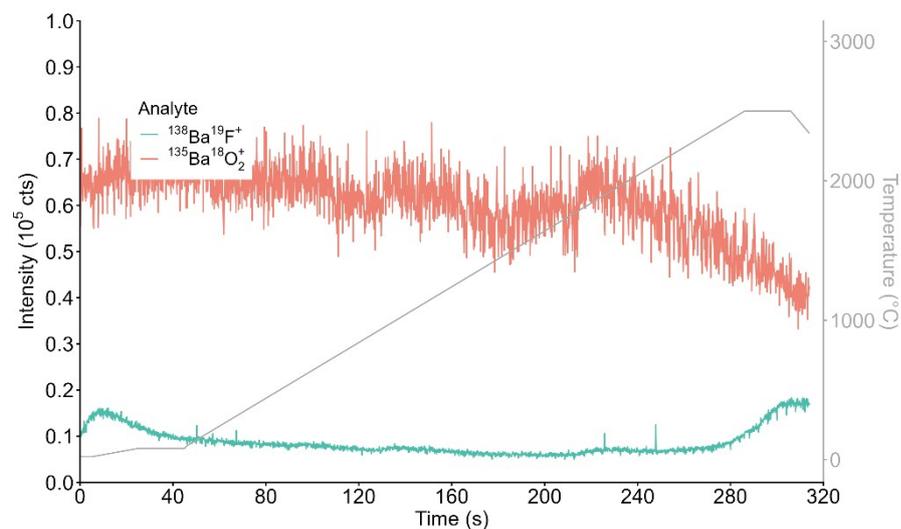


Fig. S2: ETV/ICP-QQQ-MS time scan of an empty graphite boat acquired in MS/MS scan mode (as blank). The CRC was pressured with an oxygen gas flow of 0.03 mL min⁻¹. The ETV temperature program is shown in grey.