



Supplementary figures

Sfig. 1. (a) Calibration curves for Pb/FITC nanoparticles: continuous flow after digestion in 10 μ L,

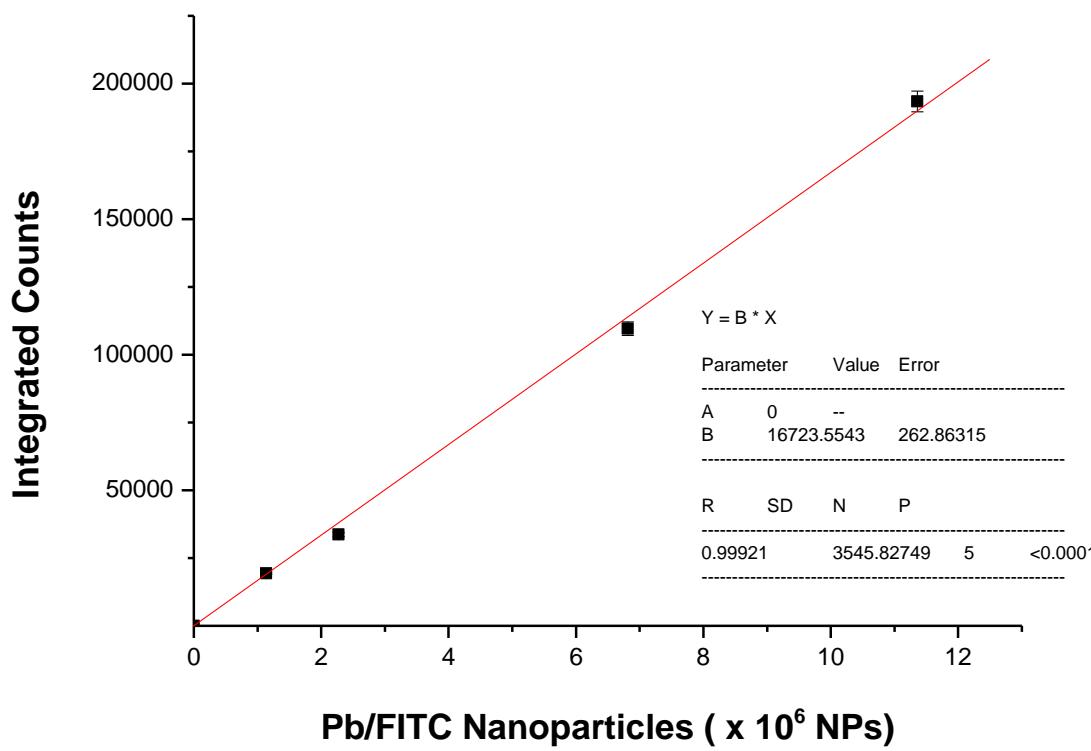

Sfig. 1. (b) calibration curves for Cd/RhBITC nanoparticles in 10 μ L with particle counting mode

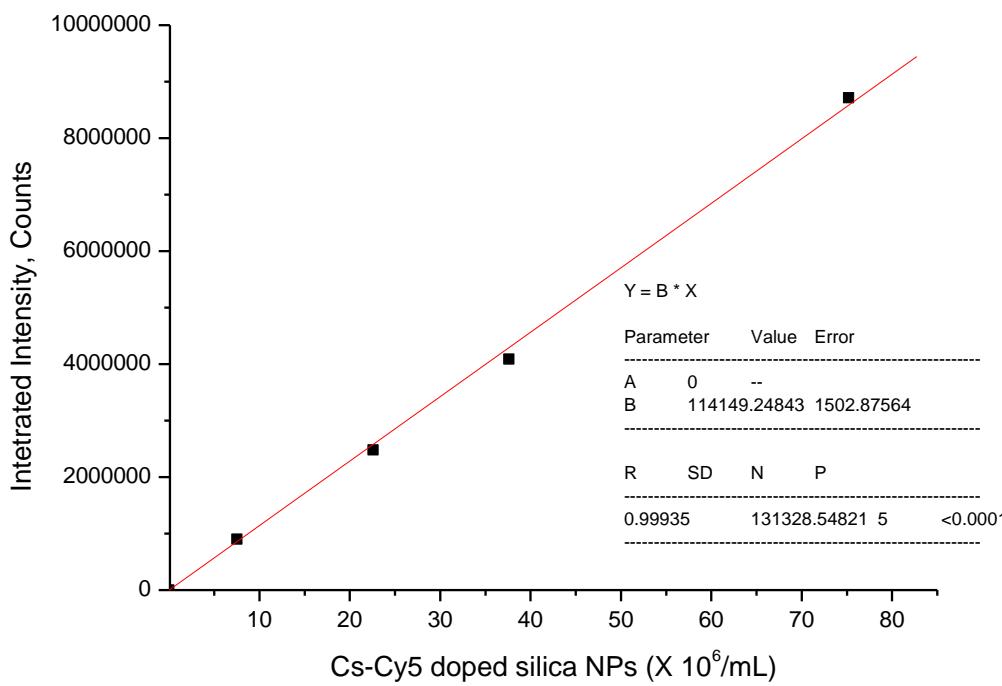

Sfig. 1. (c) calibration curves for Cs/Cy5 nanoparticles with particle counting mode

