

Electronic Supplementary Information

Simple Fabrication of Magnetically-Separable and Highly-Stable Enzyme System Based on Crosslinked Enzyme Aggregates Shipped in Magnetite-Coated Hierarchically-Ordered Mesocellular Mesoporous Silica

Jinwoo Lee,^{¶^a} Hyon Bin Na,^{¶^b} Byoung Chan Kim,^c Jin Hyung Lee,^d Byoungsoo Lee,^e Ja Hun Kwak,^f Yosun Hwang,^g Je-Geun Park,^g Man Bock Gu,^d Jaeyun Kim,^b Jin Joo,^b Chae-Ho Shin,^h Jay W. Grate,^f Taeghwan Hyeon^{*^b} and Jungbae Kim^{*^e}

^a Department of Chemical Engineering/School of Environmental Science and Engineering, Pohang University of Science and Technology, Kyungbuk, 790-784 (Korea); E-mail: jinwoo03@postech.ac.kr

^b National Creative Research Initiative Center for Oxide Nanocrystalline Materials and School of Chemical Engineering, Seoul National University, Seoul 151-744 (Korea); E-mail: thyeon@plaza.snu.ac.kr

^c Institut Pasteur Korea, Songnam-si, Gyeonggi-do 463-400 (Korea)

^d College of Life Sciences and Biotechnology, Korea University, Seoul 136-701 (Korea)

^e Department of Chemical and Biological Engineering, Korea University, Seoul 136-701 (Korea); E-mail: jbkim3@korea.ac.kr

^f Pacific Northwest National Laboratory, Richland, WA 99352 (USA)

^g Department of Physics, Sungkyunkwan University, Suwon 440-746 (Korea)

^h Department of Chemical Engineering, Chungbuk National University, Cheongju, Chungbuk 360-763 (Korea)

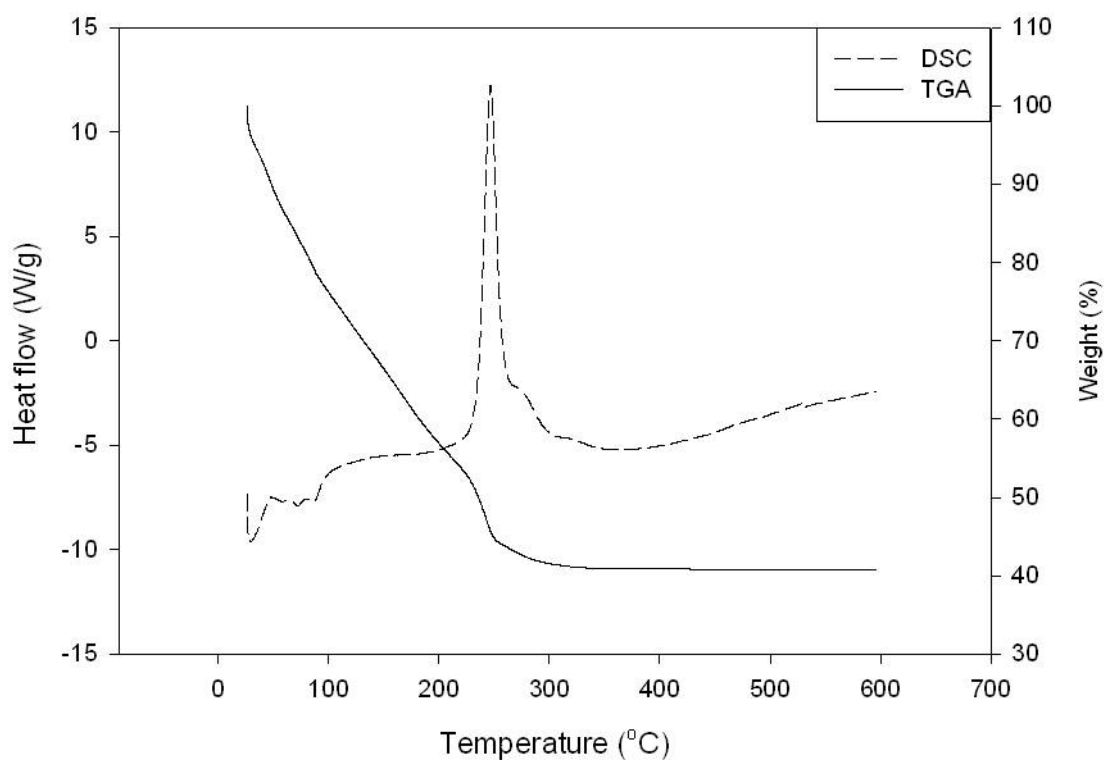


Fig. S1 Thermogravimetric analysis (TGA) and differential scanning calorimetry (DSC) curves of iron propionate/HMMS composite.

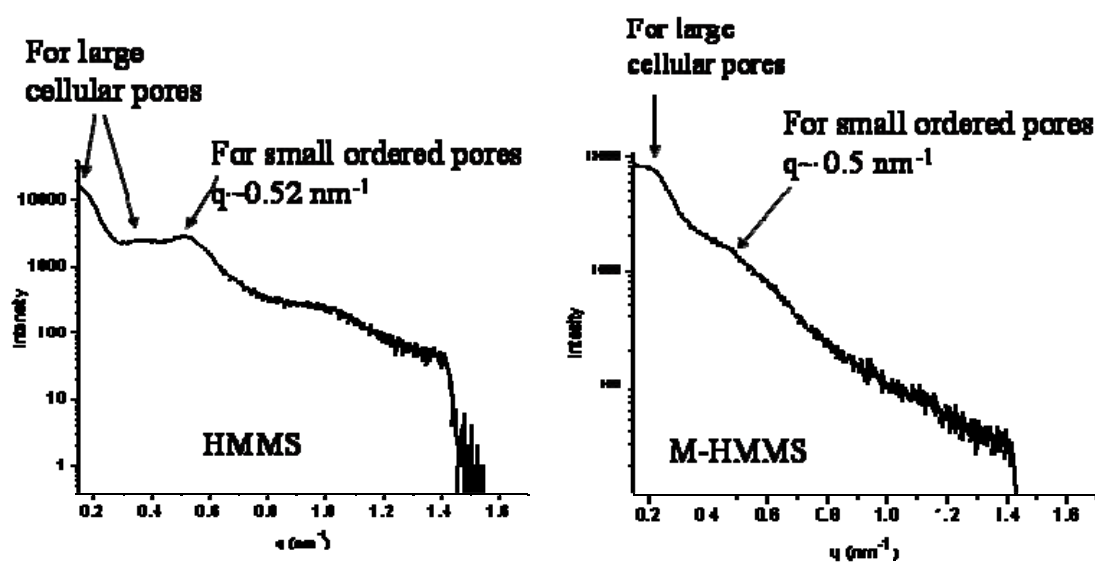


Fig. S2 Small-angle X-ray scattering data of HMMS and M-HMMS.

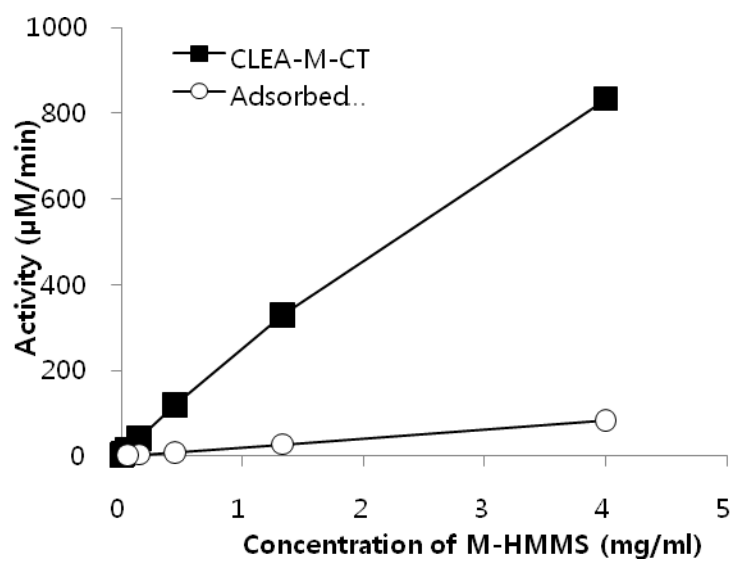


Fig. S3 Correlation between initial rates of immobilized CT and the amount of enzyme, represented by the weight of M-HMMS.