

Electronic Supplementary Information (ESI) available:

(1) Preparation of GO suspension with various concentrations



Fig. S1 GO suspension from left to right : 2 mg/ml, 1 mg/ml, 0.5 mg/ml, 0.1 mg/ml, 0.05 mg/ml.

(3) PDMS stamp for imprinting

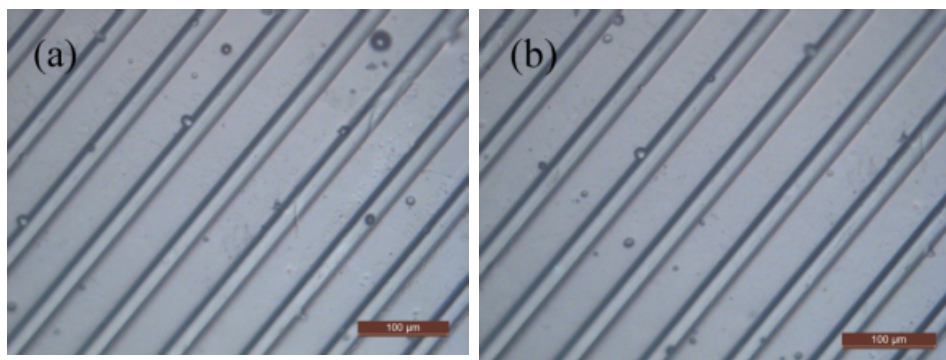
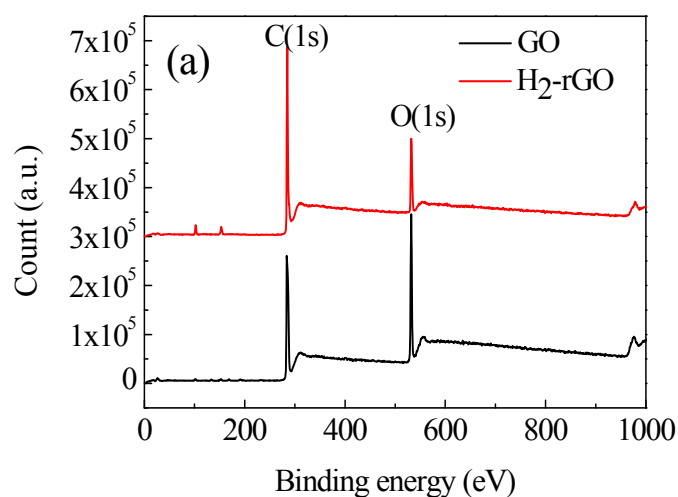


Fig. S2 Optical image of PDMS before (a) and after (b) imprinting process

(2) XPS characterization of GO and rGO



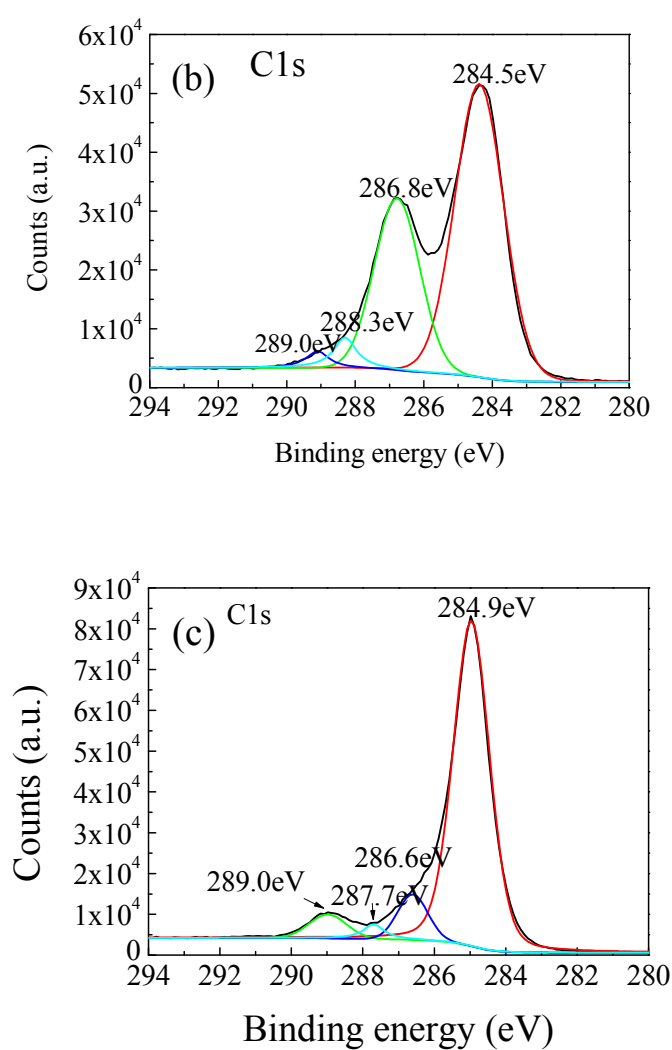


Fig. S2 (a) XPS survey of as-made GO and rGO, (b) C1s spectra of GO, (c) C1s spectra of rGO