

Electric Supplementary Information

On-Chip pH Measurement Using Functionalized Gel-Microbeads Positioned by Optical Tweezers

Hisataka Maruyama, Fumihito Arai and Toshio Fukuda

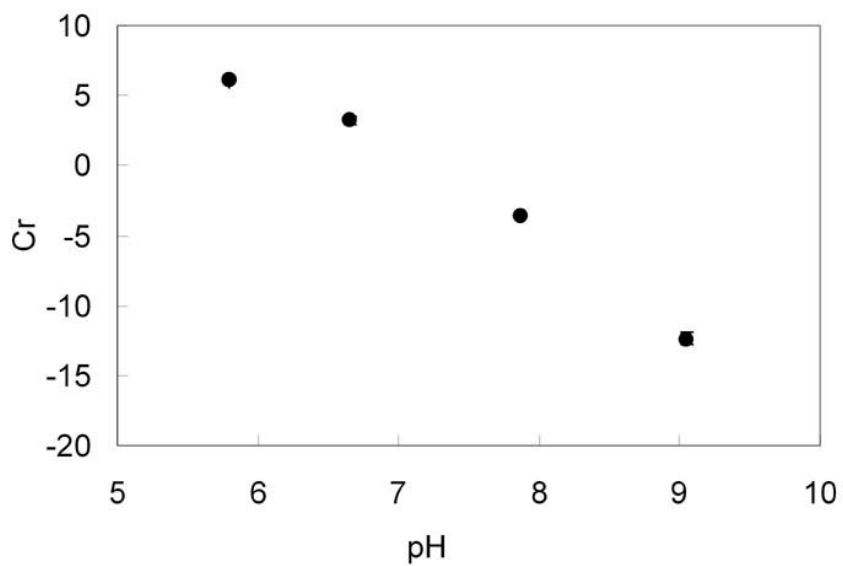


Fig. S1 Calibration result of pH with Cr.

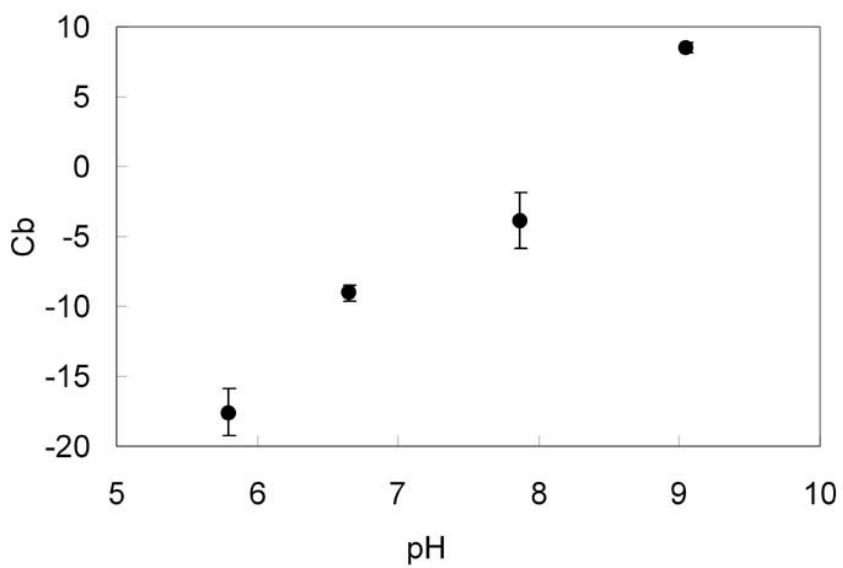


Fig. S2 Calibration results of pH with Cb.