

Supporting Information

Bulk- and Surface-Modified Combinable PDMS Capillary Sensor Array as Easy-to-use Multi Sensing Device with Enhanced Sensitivity for Discriminating Elevated Concentration Component in Serum Sample

Yuji Fujii, Terence G. Henares, Kunio Kawamura, Tatsuro Endo, and Hideaki Hisamoto*

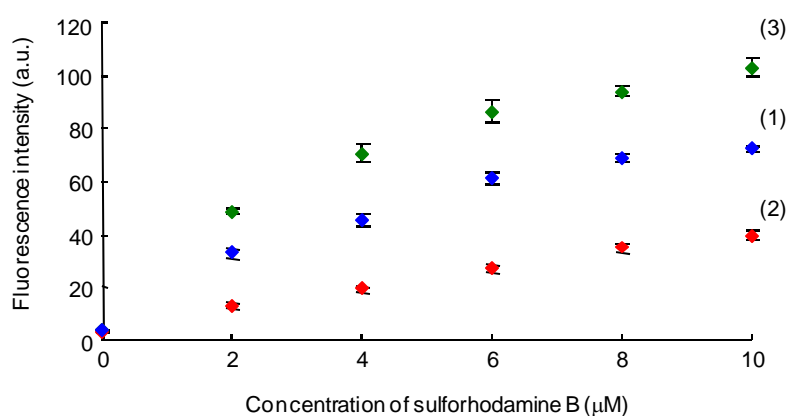


Figure S1 Calibration curves of sulforhodamine B solutions using different CPCs.
(1)Conventional CPC, (2)Bulk modified CPC, (3)Surface modified CPC
(Error bar represents relative standard deviation (n=3))