

SUPPLEMENTAL CONTENT

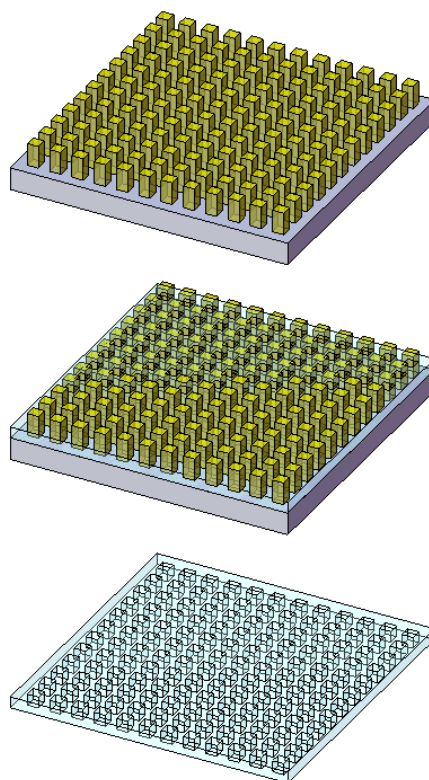


Fig. S1 – Fabrication process of PDMS grid from casting on SU-8 pillars from mold master.

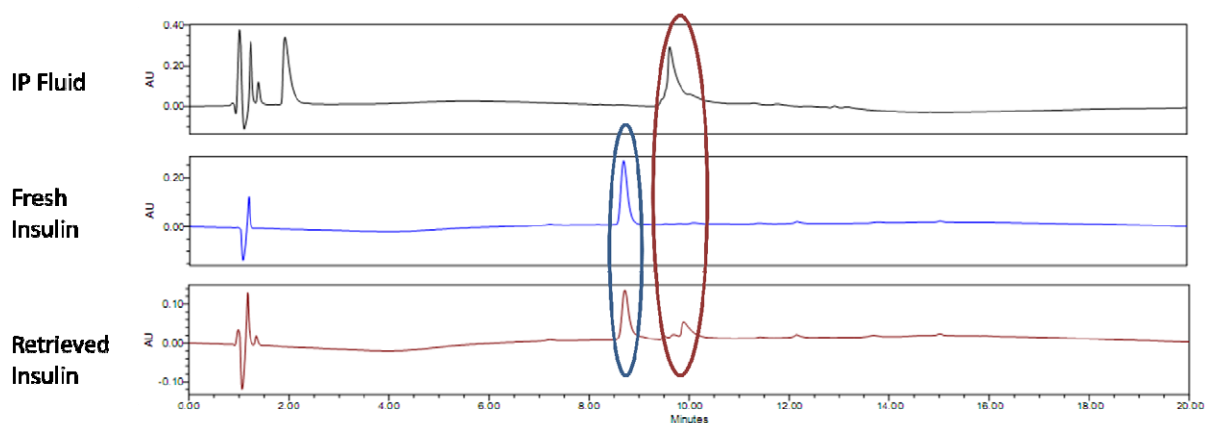


Fig. S2 – RP-HPLC chromatogram of soluble insulin from retrieved microdevices after 15 days of in vivo implantation compared with fresh human recombinant insulin and intraperitoneal (IP) fluid with endogenous proteins.