

Electronic Supplementary Information


A Bubble-based Microfluidic Gas Sensor for Gas Chromatographs

Ashrafuzzaman Bulbul and Hanseup Kim

Electrical and Computer Engineering, University of Utah

Abstract:

This supplementary information includes some additional information to support the original data presented in the original manuscript.

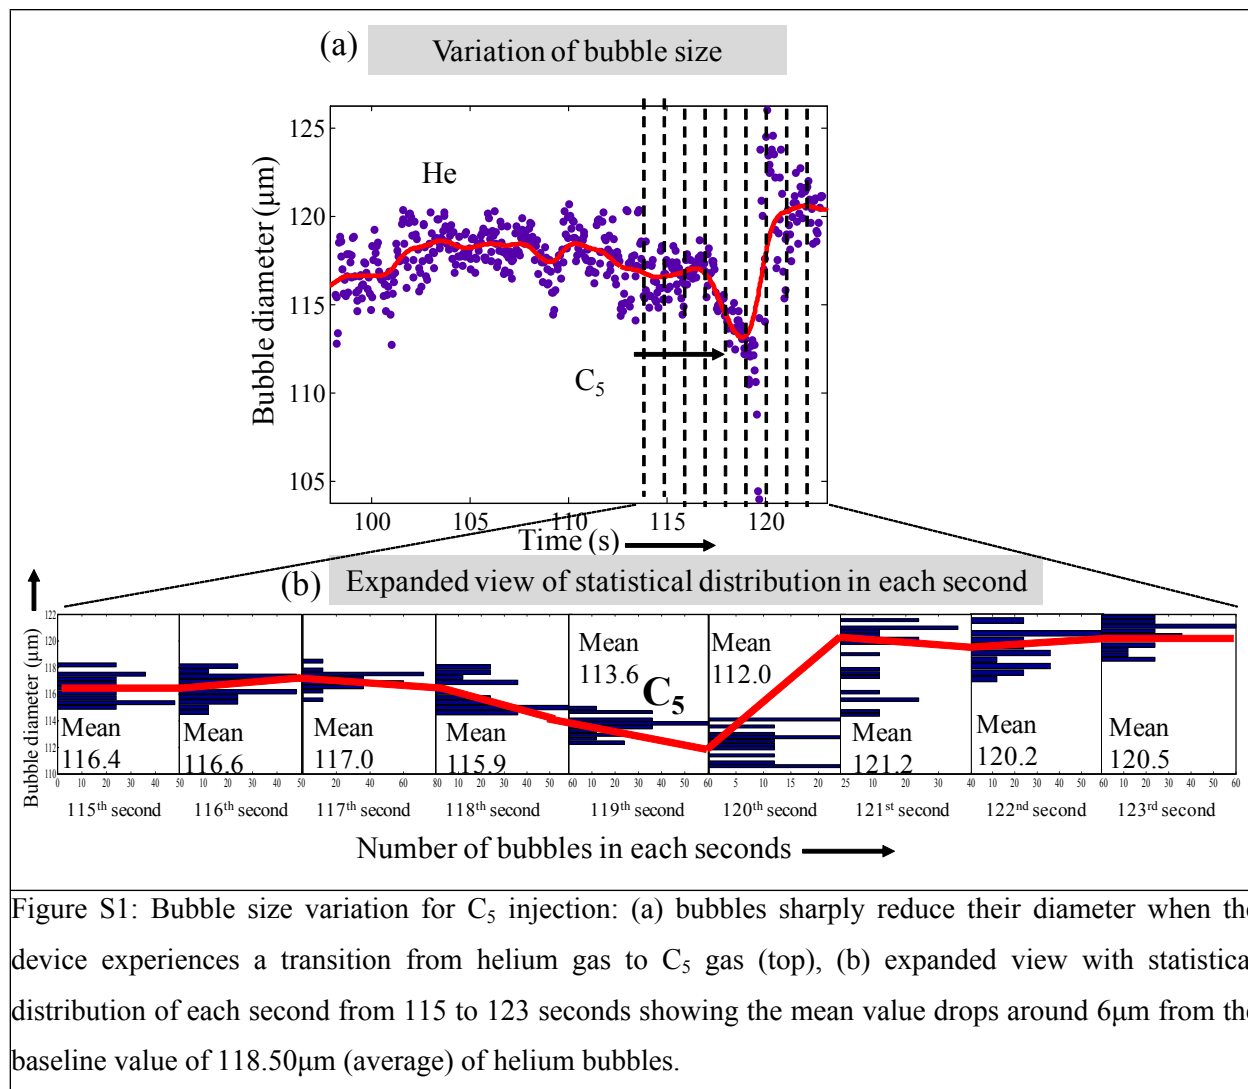

Stability over time

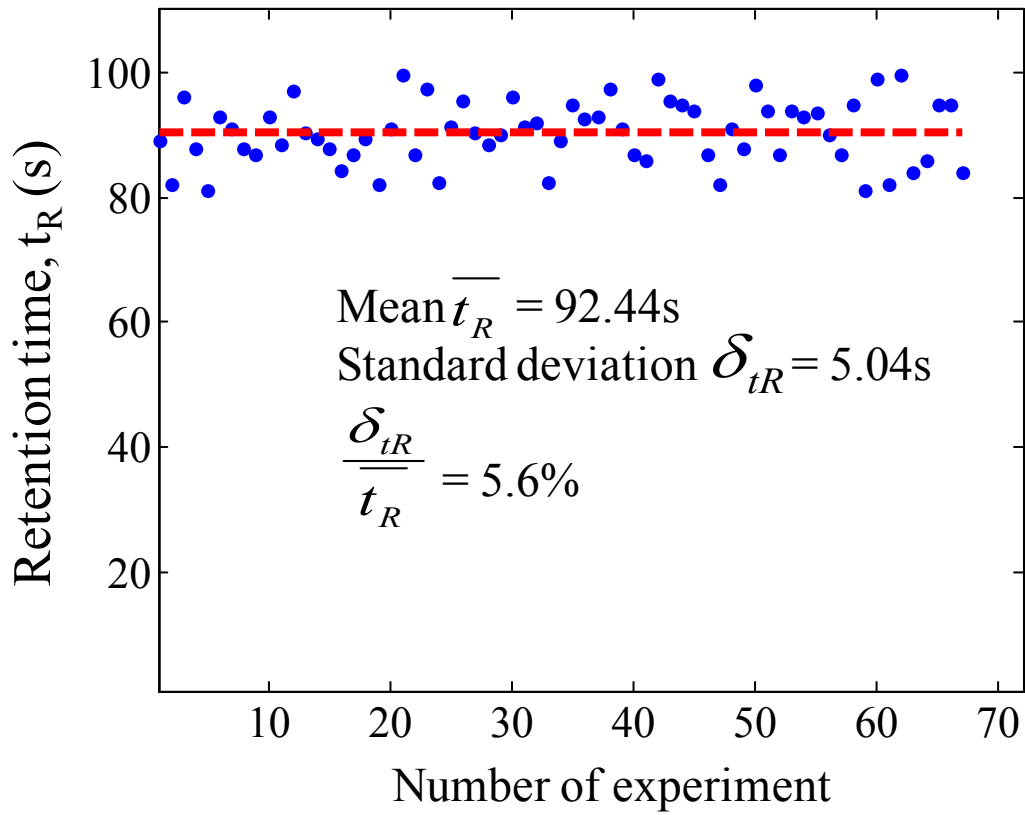


Figure S2: Variation of retention time over 67 tests for same amount of injection volume (0.001 μL) showing only 5.60% variations around the mean retention time of 92.44s.