

Supplementary Information

pH-sensitive spectrophotometric control of nilutamide in an automatic micro-flow system

Mélodie M. Carvalho, David S. M. Ribeiro, João L. M. Santos, João A. V. Prior*

Requimte, Laboratory of Applied Chemistry, Department of Chemical Sciences, Faculty of Pharmacy, University of Porto, Rua de Jorge Viterbo Ferreira n.º 228, 4050-313, Porto, Portugal.

e-mail address: joaoavp@ff.up.pt; Tel.: 00351 220 428 670

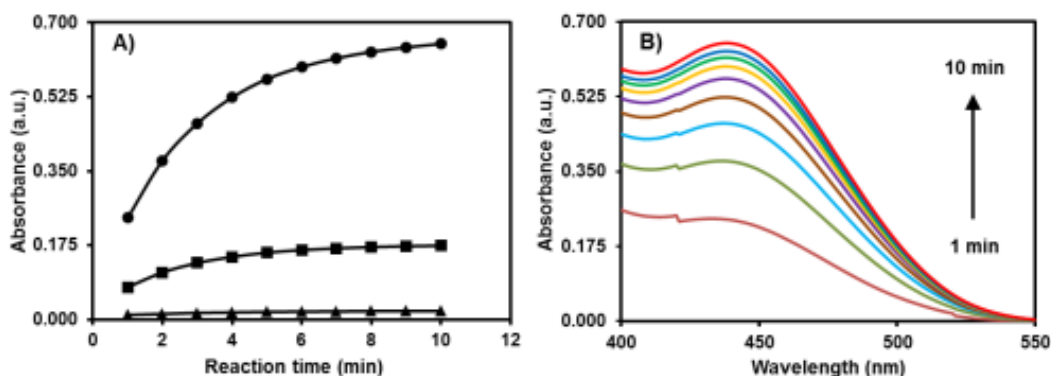


Figure 1, supplementary material. (A): Influence of reaction time on the analytical signal of different nilutamide concentrations ($\blacktriangle$ – 1 mg L⁻¹; $\blacksquare$ – 10 mg L⁻¹; $\bullet$ – 40 mg L⁻¹); (B): Absorption spectra of nilutamide solution (40 mg L⁻¹) in function of reaction time.

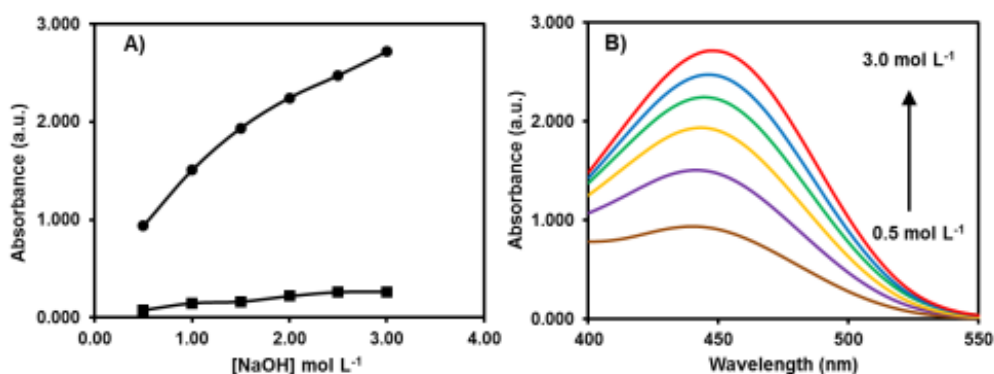


Figure 2, supplementary material. (A): Influence of sodium hydroxide concentration on the analytical signal of different nilutamide concentrations ($\blacksquare$ – 5 mg L⁻¹; $\bullet$ – 50 mg L⁻¹); (B): Absorption spectra of nilutamide solution (50 mg L⁻¹) in the presence of different sodium hydroxide concentrations.