


# Peking University Mass Spectrometry Sample Analysis Report

## Analysis Info

Analysis Name 13100414\_20131016\_000003.d  
Sample 2  
Comment ESI Positive

Acquisition Date 10/16/2013 3:57:18 PM  
Instrument Bruker Apex IV FTMS  
Operator Peking University

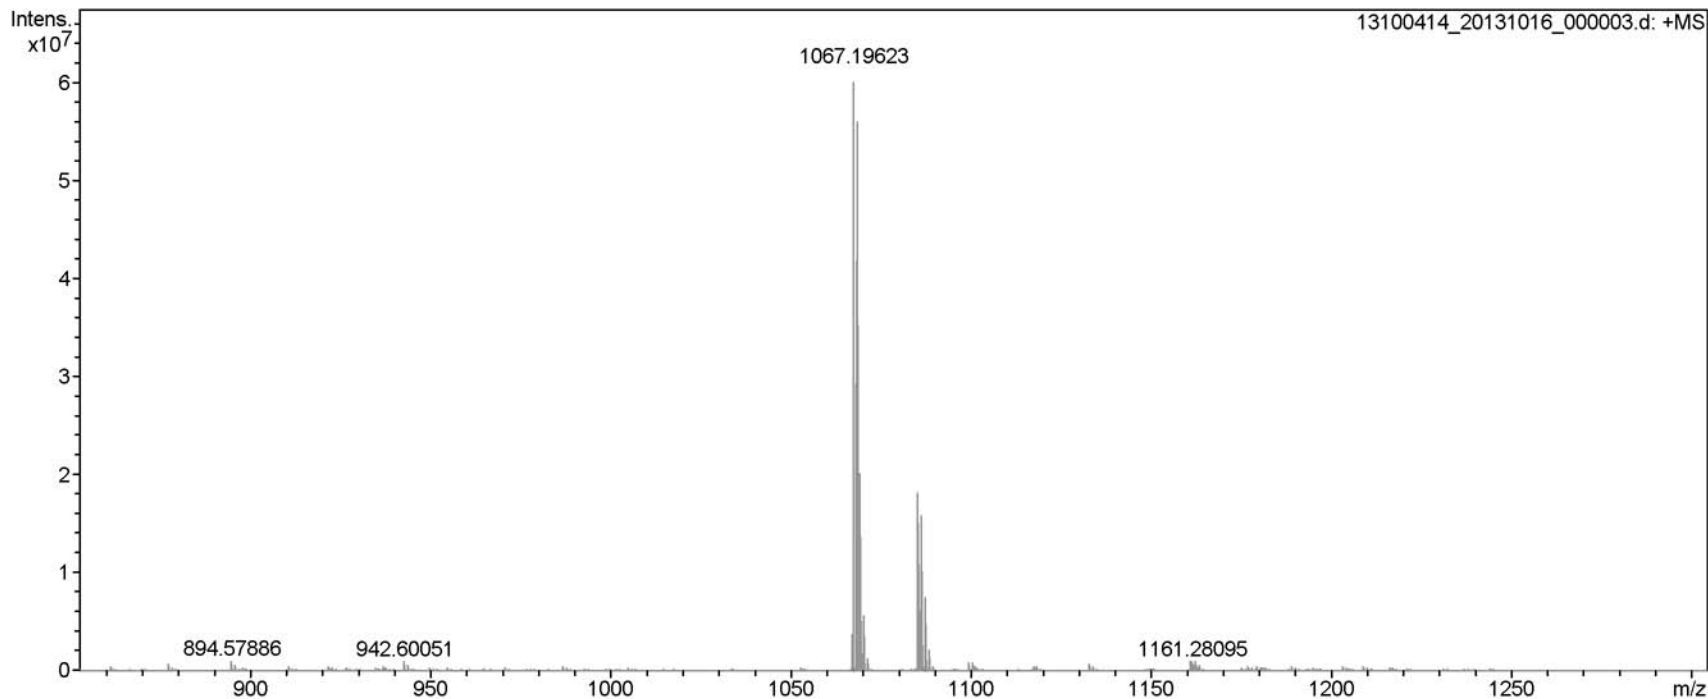

13100414\_20131016\_000003.d: +MS

Meas. m/z	#	Formula	Score	m/z	err [mDa]	err [ppm]	mSigma	rdb	e <sup>-</sup> Conf	N-Rule
1067.19623	1	C <sub>79</sub> H <sub>27</sub> N <sub>2</sub> O <sub>4</sub>	100.00	1067.19653	0.3	0.3	28.9	67.5	even	ok