


Supplementary information

(1) Supplementary Fig. S1

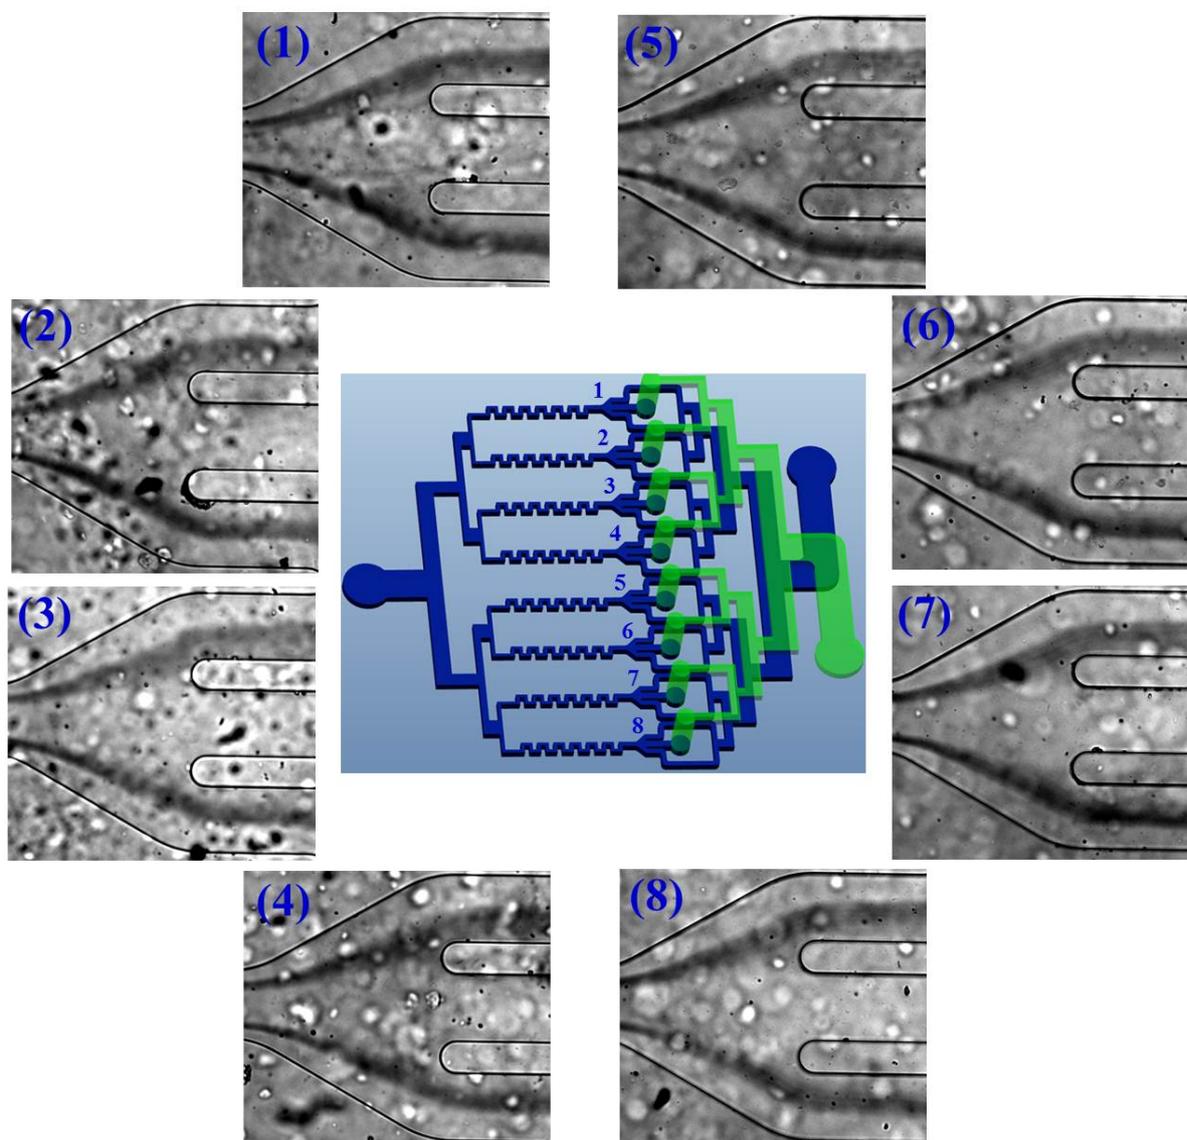

Supplementary Fig. S1 Bright field images at each outlet bifurcation in the parallel device. The uniform streamline splitting and blood cells filtration at each outlet validate our parallelization design considerations.