

Supplementary Information

The infrared absorbance spectra of the silicone samples prepared for the microbiological testing, in addition to an untreated silicone sample, obtained by ATR.

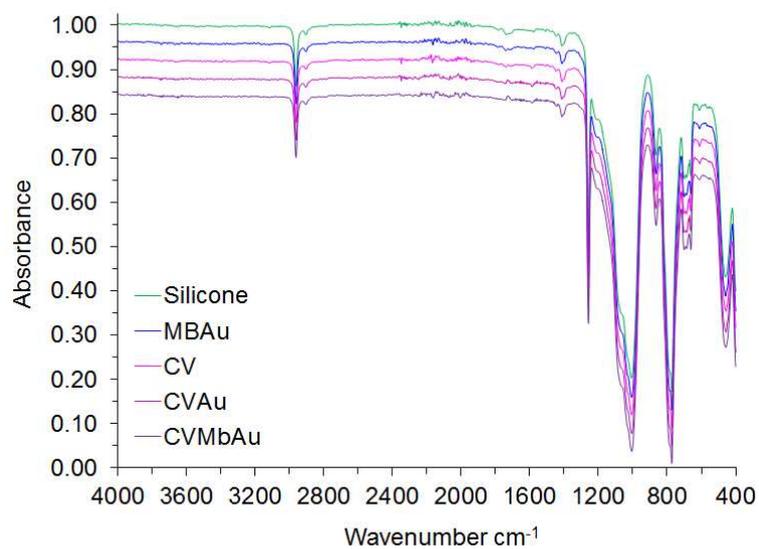


Figure 1: Supplementary Information: IR absorbance spectra of modified and untreated silicone samples measured within the range 4000 - 400 cm⁻¹