

Supporting Information

Hemocompatibility of Chitosan/poly(acrylic acid) Grafted Polyurethane Tubing

*Hyun-Su Lee^{a,b,c}, Nancy Tomczyk^a, Judith Kandel^d, Russell J. Composto^{b,c}, and David M.
Eckmann^{a,c,*}*

^aDepartment of Anesthesiology and Critical Care, ^bDepartment of Materials Science and Engineering, ^cInstitute for Medicine and Engineering, ^dDepartment of Bioengineering, University of Pennsylvania, Philadelphia, Pennsylvania 19104, United States

*Correspondence should be addressed to:

David M. Eckmann, Ph.D., M.D.

Department of Anesthesiology and Critical Care, University of Pennsylvania

331 John Morgan Building, 3620 Hamilton Walk

Philadelphia, PA 19104-6802, USA.

Tel.: +1 215 349 5348; fax: +1 215 349 5078.

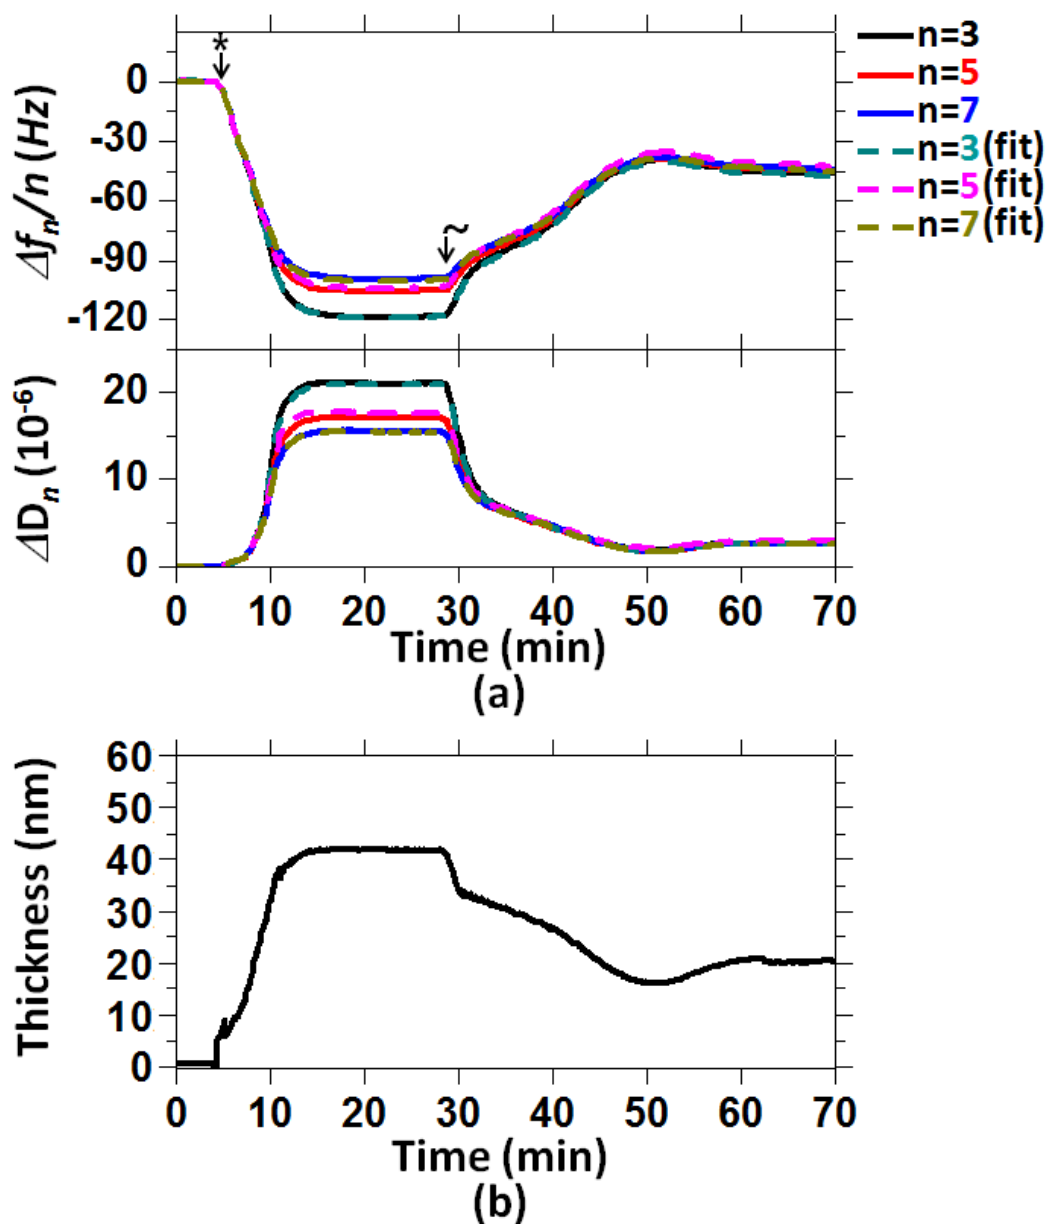


Figure. S1. (a) Simulated and experimental curves for $\Delta f_n/n$ ($n = 3, 5, 7$) and ΔD_n versus time for exposure (*) of SiO_2 surfaces to 50% plasma solutions, followed by exposure (˘) to saline solutions for rinsing step. The best fit between the viscoelastic model and the experimental data is shown. (b) Thickness versus time determined from the fit shown in (a).